


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072518\
 Data File : VU025625.D
 Acq On : 25 Jul 2018 09:09
 Operator : MD/SY
 Sample : BFB
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U072518DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Fri Jul 27 15:10:58 2018

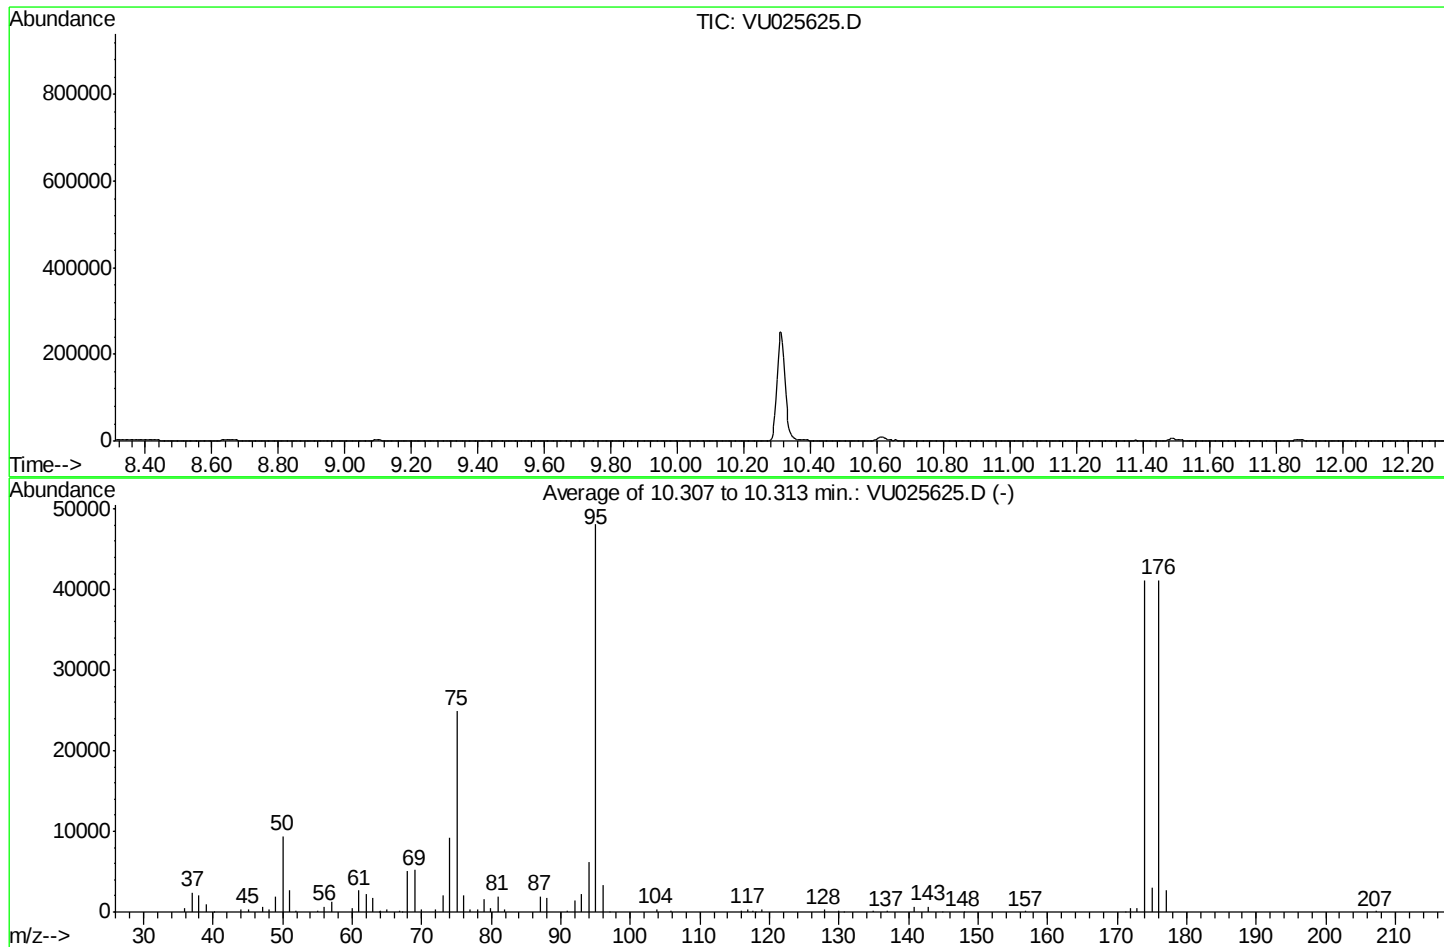

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3010

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	9430	PASS
75	95	30	60	51.9	24981	PASS
95	95	100	100	100.0	48098	PASS
96	95	5	9	6.8	3288	PASS
173	174	0.00	2	1.2	489	PASS
174	95	50	100	85.4	41088	PASS
175	174	5	9	7.3	3008	PASS
176	174	95	101	100.2	41181	PASS
177	176	5	9	6.4	2654	PASS