
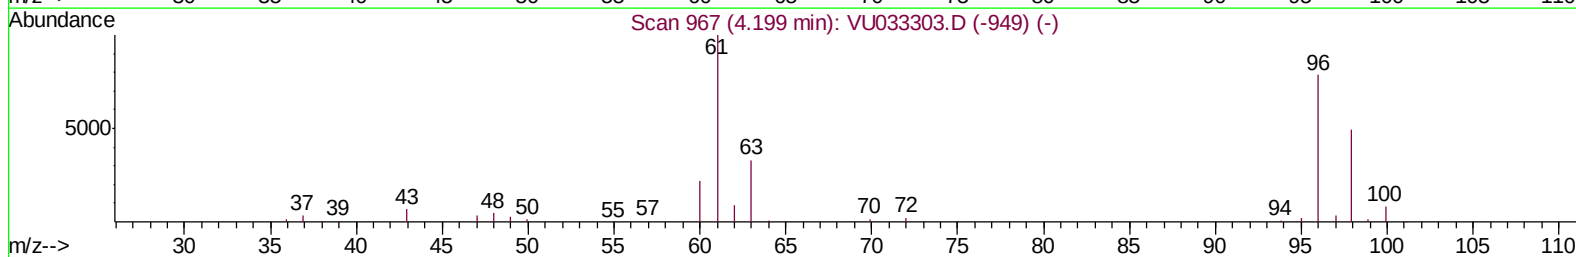
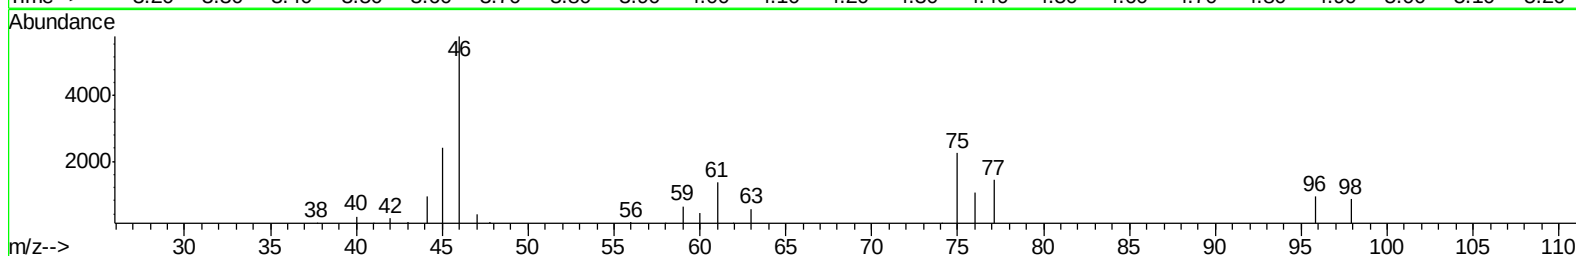


Data File : VU033431.D
Acq On : 25 Jul 2019 23:46
Operator : JC/SP
Sample : K3976-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Quant Time: Jul 26 05:55:04 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071219WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 26 05:48:12 2019
Response via : Initial Calibration

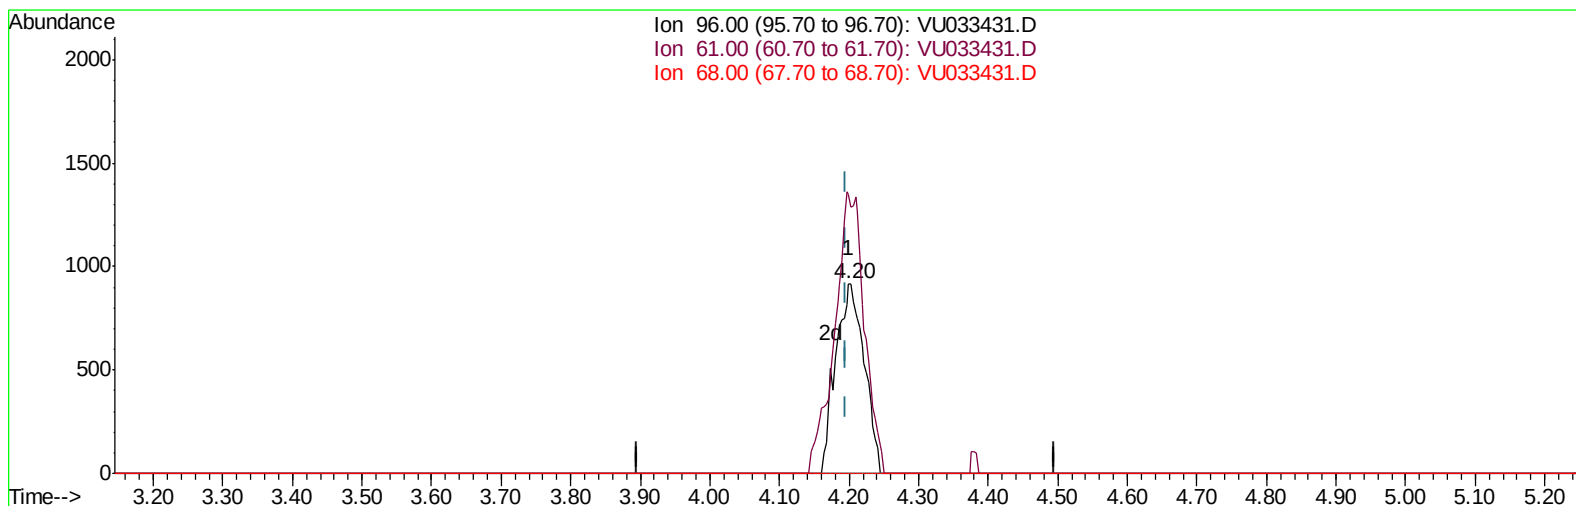

TIC: VU033431.D

(20) cis-1,2-Dichloroethene (T)

4.199min (+0.003) 1.23ug/L m

response 2624

Ion	Exp%	Act%
96.00	100	100
61.00	130.10	146.90
68.00	0.00	0.00
0.00	0.00	0.00