
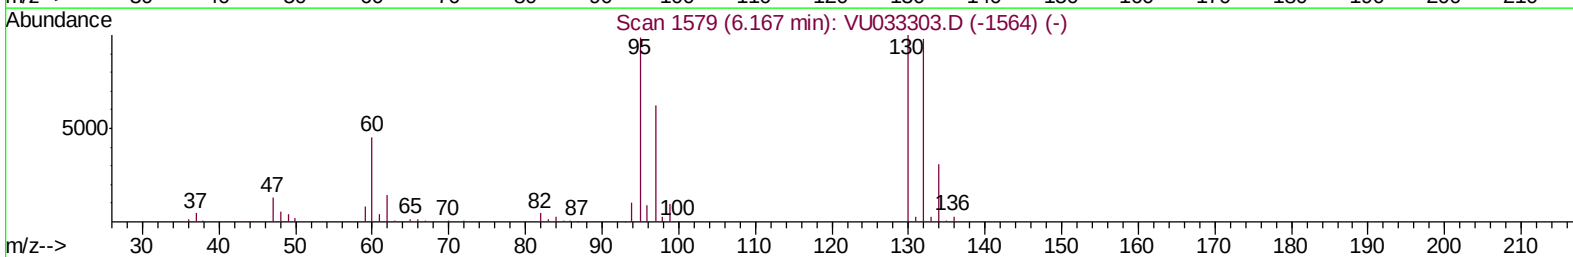
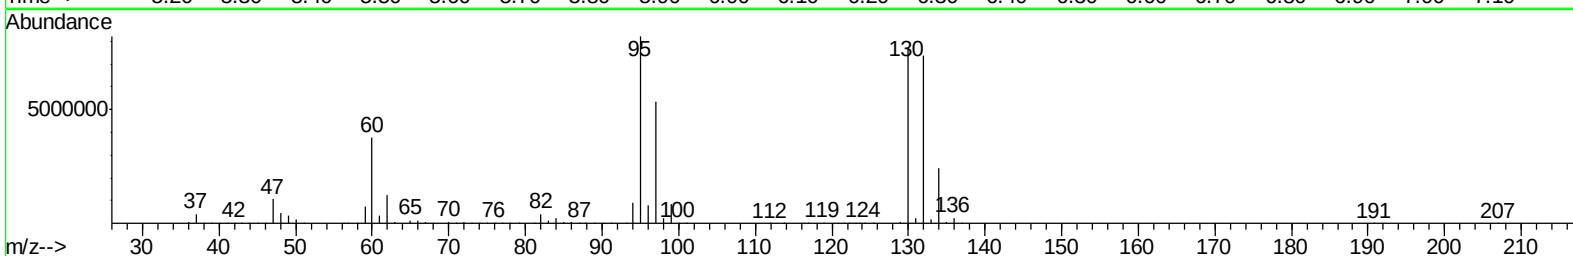


Data File : VU033435.D
Acq On : 26 Jul 2019 01:18
Operator : JC/SP
Sample : K3976-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Quant Time: Jul 26 05:55:42 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071219WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 26 05:48:12 2019
Response via : Initial Calibration

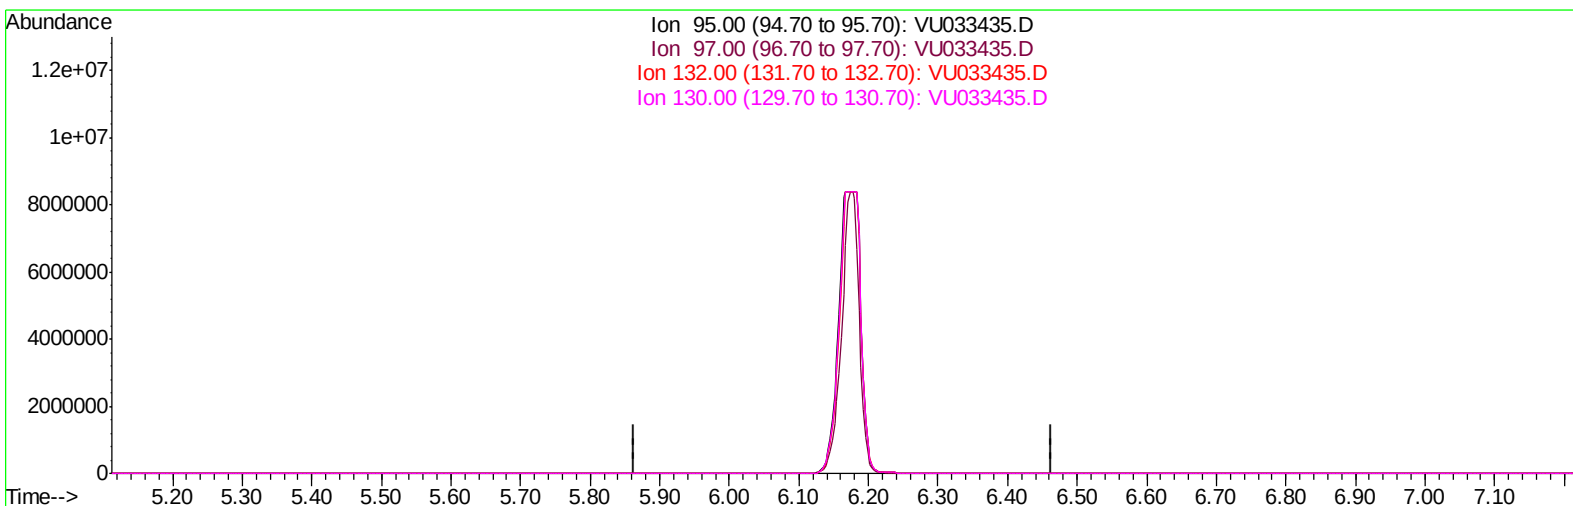

TIC: VU033435.D

(34) Trichloroethene (T)

6.164min (-6.164) 0.00ug/L

response 0

Ion	Exp%	Act%
95.00	100	0.00
97.00	62.60	0.00#
132.00	93.50	0.00#
130.00	99.60	0.00#