

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072519\
 Data File : VU033413.D
 Acq On : 25 Jul 2019 16:50
 Operator : JC/SP
 Sample : VU0725WBL02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK58

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.389	87	93	106	rVB	163754	167949	15.00%	1.939%
2	1.669	173	180	195	rVB	148354	187390	16.74%	2.164%
3	2.257	353	363	378	rVB	245078	374262	33.43%	4.321%
4	2.820	529	538	553	rVB2	3692	7473	0.67%	0.086%
5	3.019	598	600	602	rBV	137	40	0.00%	0.000%
6	3.035	602	605	610	rVB2	365	246	0.02%	0.003%
7	3.067	610	615	616	rBV3	269	249	0.02%	0.003%
8	3.151	637	641	643	rBV3	301	249	0.02%	0.003%
9	3.193	652	654	659	rBV2	373	286	0.03%	0.003%
10	3.228	664	665	667	rVB2	251	54	0.00%	0.001%
11	3.264	674	676	677	rBV	125	68	0.01%	0.001%
12	3.270	677	678	679	rBV	114	42	0.00%	0.000%
13	3.344	698	701	703	rBV2	245	194	0.02%	0.002%
14	3.463	735	738	741	rBV	180	111	0.01%	0.001%
15	3.482	741	744	747	rBV	333	260	0.02%	0.003%
16	3.534	758	760	764	rVB	417	268	0.02%	0.003%
17	3.556	764	767	769	rBV2	275	197	0.02%	0.002%
18	3.576	769	773	777	rVB2	211	202	0.02%	0.002%
19	3.656	796	798	799	rBV	241	108	0.01%	0.001%
20	3.701	809	812	816	rBV	151	105	0.01%	0.001%
21	3.720	816	818	824	rVB2	288	187	0.02%	0.002%
22	3.794	837	841	843	rVB2	242	146	0.01%	0.002%
23	3.823	848	850	854	rVB	134	84	0.01%	0.001%
24	3.897	870	873	876	rBV3	336	229	0.02%	0.003%
25	3.958	887	892	894	rBV	250	250	0.02%	0.003%
26	4.010	904	908	910	rBV3	185	138	0.01%	0.002%
27	4.026	911	913	915	rVB2	275	120	0.01%	0.001%
28	4.042	915	918	922	rVB2	132	96	0.01%	0.001%
29	4.061	922	924	926	rBV	180	85	0.01%	0.001%
30	4.093	930	934	936	rVB2	148	86	0.01%	0.001%
31	4.151	936	952	990	rBV	97495	276375	24.68%	3.191%
32	4.620	1082	1098	1122	rBV	193167	456408	40.76%	5.270%
33	4.807	1154	1156	1158	rBV2	297	147	0.01%	0.002%
34	4.955	1199	1202	1205	rBV2	404	305	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072519\
 Data File : VU033413.D
 Acq On : 25 Jul 2019 16:50
 Operator : JC/SP
 Sample : VU0725WBL02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK58

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071219WMA.M
 Title : VOC Analysis

35	5.010	1217	1219	1221	rVB2	214	87	0.01%	0.001%
36	5.032	1221	1226	1228	rBV2	179	128	0.01%	0.001%
37	5.045	1228	1230	1231	rVB2	152	40	0.00%	0.000%
38	5.071	1236	1238	1239	rVV	234	76	0.01%	0.001%
39	5.083	1239	1242	1248	rVB	316	276	0.02%	0.003%
40	5.186	1271	1274	1278	rVB2	194	124	0.01%	0.001%
41	5.209	1278	1281	1284	rBV2	204	170	0.02%	0.002%
42	5.315	1290	1314	1342	rBV2	372723	1119628	100.00%	12.927%
43	5.743	1443	1447	1449	rBV3	259	221	0.02%	0.003%
44	5.762	1449	1453	1455	rBV2	210	155	0.01%	0.002%
45	5.865	1471	1485	1510	rBV	326712	659450	58.90%	7.614%
46	6.309	1609	1623	1650	rBV	255046	507620	45.34%	5.861%
47	6.498	1680	1682	1687	rVB2	401	232	0.02%	0.003%
48	6.546	1695	1697	1698	rBB2	201	57	0.01%	0.001%
49	6.646	1725	1728	1731	rBV	255	183	0.02%	0.002%
50	6.727	1750	1753	1756	rVB	154	109	0.01%	0.001%
51	6.746	1756	1759	1761	rBV	280	127	0.01%	0.001%
52	6.781	1767	1770	1774	rBV3	323	200	0.02%	0.002%
53	6.855	1788	1793	1795	rBV2	392	351	0.03%	0.004%
54	6.913	1808	1811	1815	rVB2	195	125	0.01%	0.001%
55	7.209	1891	1903	1927	rBV	136069	247763	22.13%	2.861%
56	7.501	1992	1994	1995	rBV	143	57	0.01%	0.001%
57	7.546	1995	2008	2038	rBV	480704	867786	77.51%	10.019%
58	7.833	2086	2097	2117	rBV	93972	164123	14.66%	1.895%
59	8.071	2167	2171	2178	rVB2	335	309	0.03%	0.004%
60	8.099	2178	2180	2181	rBV	214	104	0.01%	0.001%
61	8.157	2193	2198	2204	rBV3	781	1140	0.10%	0.013%
62	8.215	2210	2216	2219	rBV4	605	557	0.05%	0.006%
63	8.231	2219	2221	2223	rVB2	193	62	0.01%	0.001%
64	8.296	2230	2241	2271	rBV	299120	547160	48.87%	6.317%
65	8.675	2357	2359	2364	rVB	246	121	0.01%	0.001%
66	8.704	2365	2368	2369	rBV2	296	159	0.01%	0.002%
67	8.759	2383	2385	2388	rBV2	189	86	0.01%	0.001%
68	8.890	2424	2426	2430	rVB2	306	175	0.02%	0.002%
69	9.019	2464	2466	2468	rBV	234	112	0.01%	0.001%
70	9.074	2470	2483	2511	rBV	494682	854301	76.30%	9.864%
71	9.312	2555	2557	2558	rVB	229	63	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072519\
 Data File : VU033413.D
 Acq On : 25 Jul 2019 16:50
 Operator : JC/SP
 Sample : VU0725WBL02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK58

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071219WMA.M
 Title : VOC Analysis

72	9.370	2568	2575	2580	rBV4	1064	1460	0.13%	0.017%
73	9.447	2596	2599	2600	rBV	341	145	0.01%	0.002%
74	9.479	2607	2609	2615	rVB2	471	314	0.03%	0.004%
75	9.501	2615	2616	2620	rBV2	128	71	0.01%	0.001%
76	9.521	2620	2622	2623	rBV	251	119	0.01%	0.001%
77	9.723	2683	2685	2688	rBV	191	93	0.01%	0.001%
78	9.932	2747	2750	2751	rBV2	156	92	0.01%	0.001%
79	9.964	2759	2760	2763	rVB	235	84	0.01%	0.001%
80	9.996	2767	2770	2773	rBV	221	147	0.01%	0.002%
81	10.099	2800	2802	2804	rVB	270	90	0.01%	0.001%
82	10.263	2851	2853	2855	rBV	222	85	0.01%	0.001%
83	10.312	2866	2868	2871	rVB	292	129	0.01%	0.001%
84	10.363	2881	2884	2886	rBV	186	131	0.01%	0.002%
85	10.414	2888	2900	2920	rBV	377144	608625	54.36%	7.027%
86	10.566	2944	2947	2950	rBV	196	130	0.01%	0.002%
87	10.582	2950	2952	2953	rBV	279	112	0.01%	0.001%
88	10.733	2997	2999	3000	rBV	272	121	0.01%	0.001%
89	10.839	3030	3032	3035	rVB2	305	145	0.01%	0.002%
90	10.881	3042	3045	3049	rBV3	247	202	0.02%	0.002%
91	11.003	3080	3083	3089	rBV3	248	295	0.03%	0.003%
92	11.183	3137	3139	3142	rVB	362	137	0.01%	0.002%
93	11.202	3142	3145	3147	rBV2	242	129	0.01%	0.001%
94	11.250	3156	3160	3161	rBV2	245	170	0.02%	0.002%
95	11.469	3216	3228	3249	rBV	498798	783768	70.00%	9.049%
96	11.845	3332	3345	3374	rBV	496742	816210	72.90%	9.424%
97	12.151	3438	3440	3442	rBV3	440	198	0.02%	0.002%


Sum of corrected areas: 8661048

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU072519\
Data File : VU033413.D
Acq On : 25 Jul 2019 16:50
Operator : JC/SP
Sample : VU0725WBL02
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK58

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

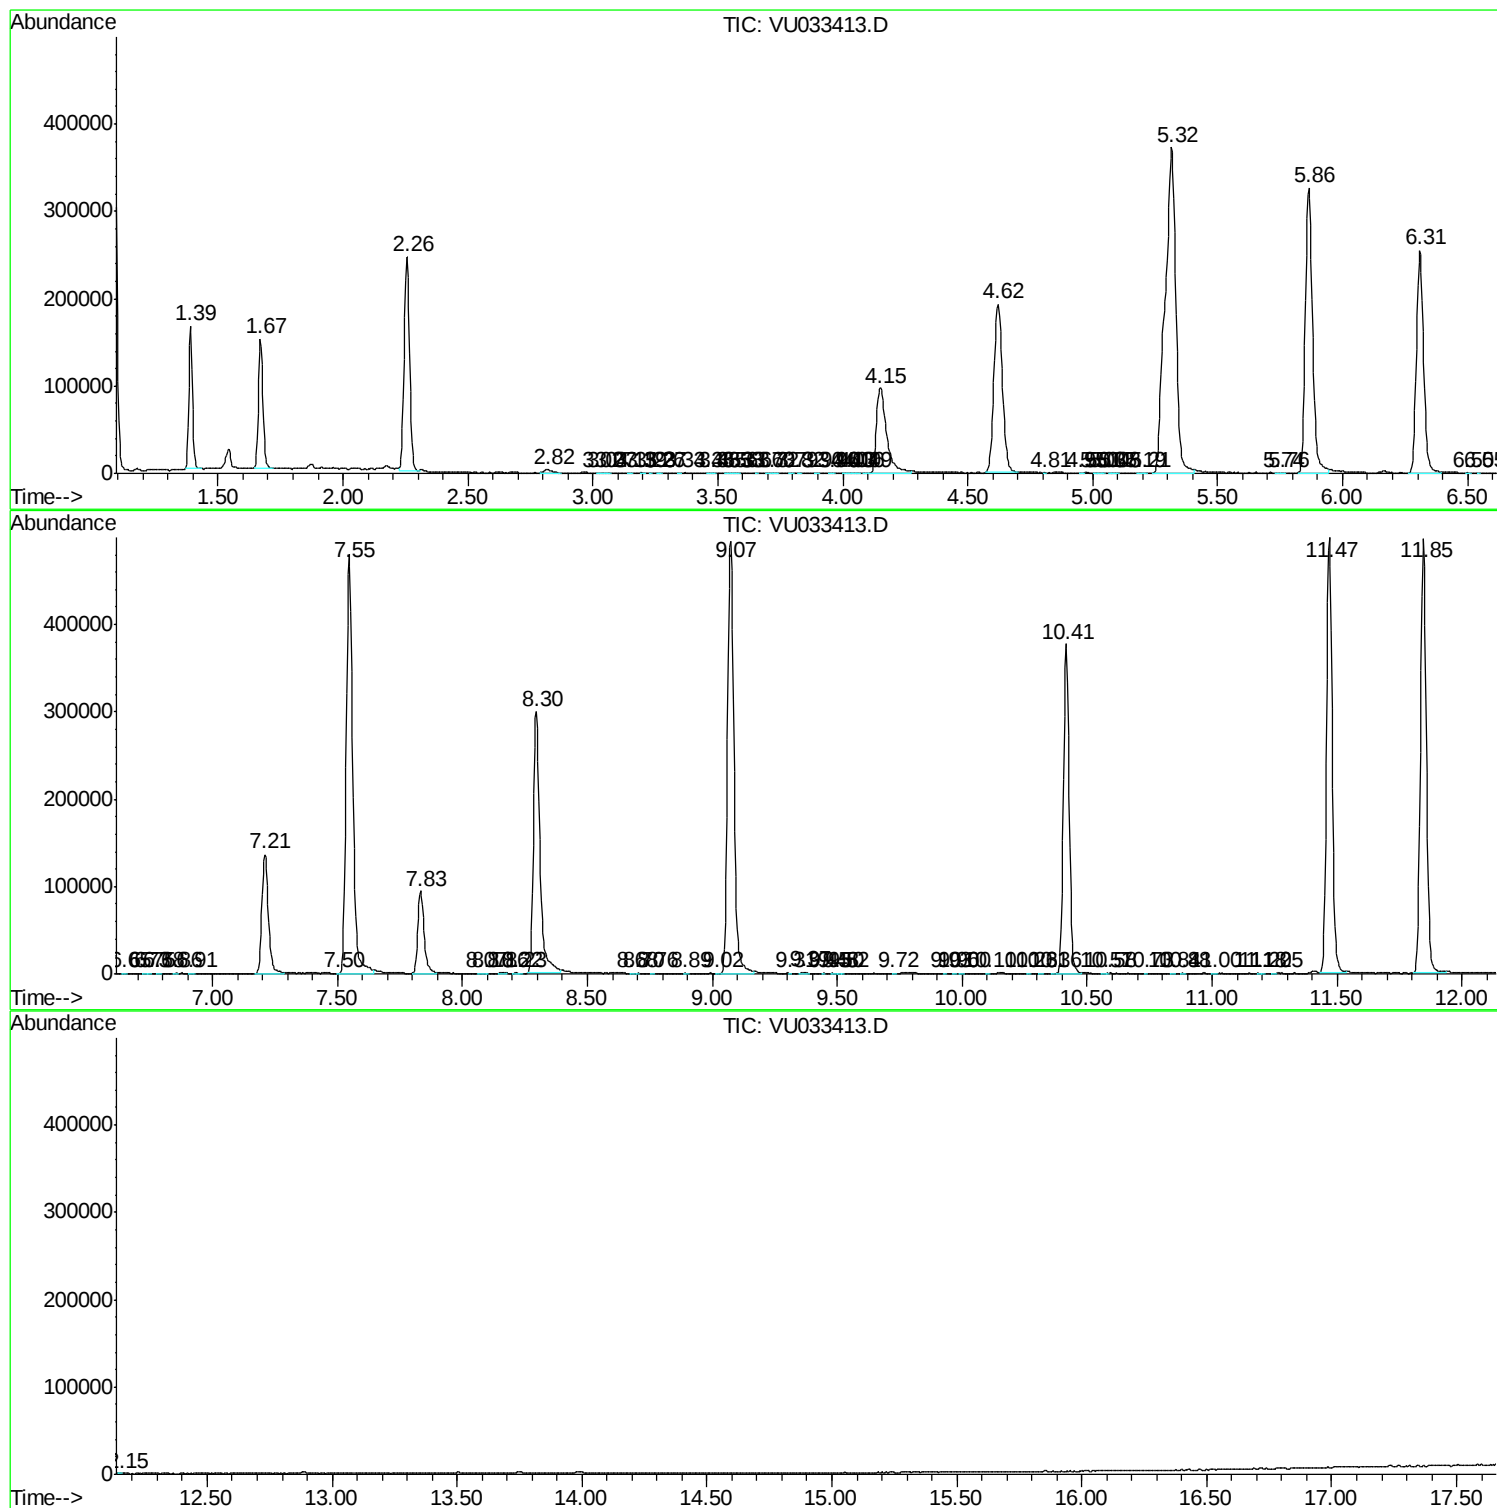

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU072519\
Data File : VU033413.D
Acq On : 25 Jul 2019 16:50
Operator : JC/SP
Sample : VU0725WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK58

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU072519\
Data File : VU033413.D
Acq On : 25 Jul 2019 16:50
Operator : JC/SP
Sample : VU0725WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK58

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc