


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU072519\
 Data File : VU033393.D
 Acq On : 25 Jul 2019 08:19
 Operator : JC/SP
 Sample : BFB38
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB38

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071219WMA.M
 Title : VOC Analysis
 Last Update : Fri Jul 26 08:22:06 2019

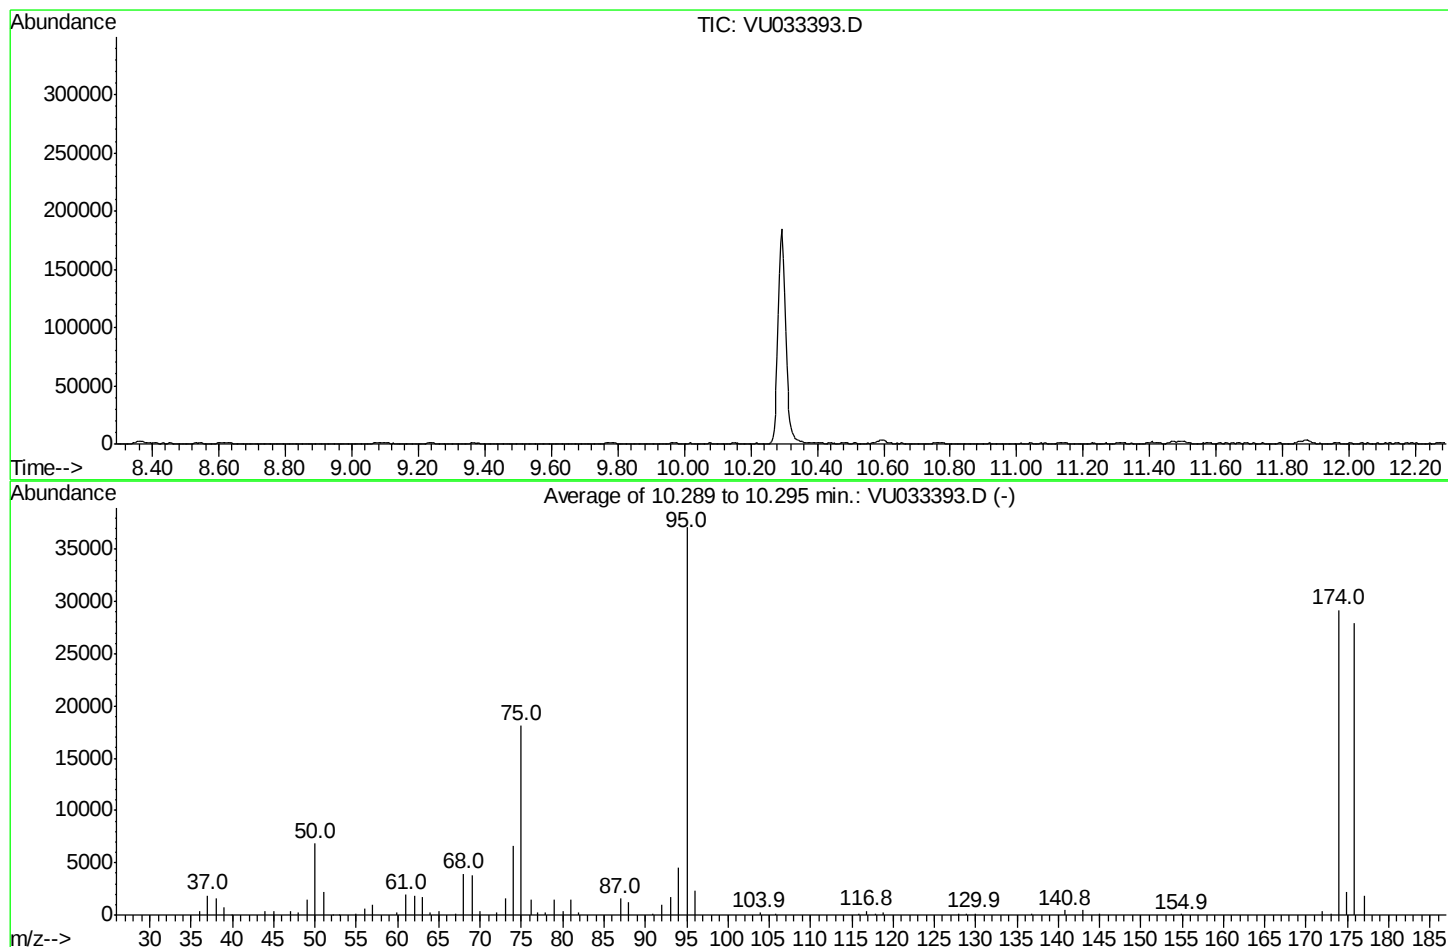

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2850

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	6836	PASS
75	95	30	80	48.8	18106	PASS
95	95	100	100	100.0	37104	PASS
96	95	5	9	6.3	2323	PASS
173	174	0.00	2	0.6	184	PASS
174	95	50	120	78.6	29176	PASS
175	174	5	9	7.8	2263	PASS
176	174	95	101	95.6	27901	PASS
177	176	5	9	6.5	1820	PASS

Scan 2850 (10.254 min): VU033393.D
BFB38

m/z	Abundance
40.00	148.0
43.90	265.0

Instrument :
MSVOA_U
ClientSampleId :
BFB38

m/z	Abundance
35.90	327.0
37.00	1865.0
38.00	1583.0
39.00	692.0
39.90	168.0
44.00	599.0
45.00	352.0
47.10	331.0
48.00	173.0
49.00	1535.0
50.00	6769.0
51.00	2202.0
52.10	109.0
52.90	104.0
54.90	159.0
56.00	578.0
57.00	966.0
59.90	299.0
61.00	1918.0
62.00	1785.0
63.00	1627.0
64.00	198.0
65.00	379.0
67.00	107.0
68.00	3789.0
69.00	3705.0
70.00	301.0
72.00	247.0
73.00	1497.0
74.00	6501.0
75.00	17664.0
76.10	1371.0
77.00	275.0
77.90	182.0
78.90	1549.0
80.00	364.0
80.90	1566.0
81.90	234.0
86.90	1469.0
87.90	1330.0
90.90	123.0
92.00	964.0
93.00	1548.0
94.10	4330.0
95.00	35968.0
96.00	2353.0
103.90	226.0
105.80	174.0
115.80	161.0
116.80	327.0
118.80	255.0
128.00	109.0
128.80	117.0
129.90	116.0
136.80	101.0
140.90	422.0
142.90	489.0
172.00	430.0
173.10	552.0
174.00	27528.0
175.00	2163.0
175.90	26064.0
177.00	1731.0

Instrument :
MSVOA_U
ClientSampleId :
BFB38

m/z	Abundance
35.90	340.0
37.00	1958.0
38.00	1713.0
39.00	698.0
39.90	200.0
44.00	616.0
45.00	391.0
47.00	324.0
47.90	222.0
49.00	1556.0
50.00	7045.0
51.00	2292.0
54.90	137.0
56.10	659.0
57.00	1062.0
60.00	277.0
61.00	1989.0
62.00	1905.0
63.00	1754.0
63.90	233.0
65.00	380.0
67.00	141.0
68.00	4086.0
69.00	3885.0
70.00	362.0
71.90	266.0
73.00	1624.0
74.00	6816.0
75.00	18560.0
76.10	1470.0
76.90	289.0
77.90	221.0
79.00	1497.0
80.00	421.0
80.90	1579.0
81.80	273.0
87.00	1558.0
87.90	1240.0
90.80	109.0
92.00	964.0
93.00	1734.0
94.00	4641.0
95.00	38232.0
96.10	2373.0
103.90	223.0
105.80	165.0
115.80	173.0
116.90	410.0
117.80	105.0
118.80	263.0
128.00	140.0
128.80	104.0
129.90	196.0
136.80	106.0
140.90	490.0
142.90	478.0
145.00	118.0
154.90	127.0
172.00	418.0
174.00	30024.0
175.00	2313.0
175.90	28872.0
177.00	1853.0

Instrument :
MSVOA_U
ClientSampleId :
BFB38

m/z	Abundance
36.00	328.0
37.00	1766.0
38.00	1580.0
39.00	663.0
39.90	216.0
44.00	552.0
45.00	382.0
47.00	292.0
47.90	262.0
49.00	1420.0
50.00	6694.0
51.00	2101.0
54.90	107.0
56.10	665.0
57.00	1077.0
60.00	284.0
61.00	1928.0
62.00	1907.0
63.00	1631.0
63.90	250.0
65.00	352.0
67.00	131.0
68.00	3971.0
69.00	3770.0
70.00	385.0
71.90	286.0
73.00	1545.0
74.00	6556.0
75.00	18096.0
76.10	1404.0
76.90	266.0
77.90	238.0
79.00	1336.0
80.00	432.0
80.90	1408.0
81.80	291.0
87.00	1616.0
87.90	1117.0
92.00	877.0
93.00	1748.0
94.00	4519.0
95.00	37112.0
96.10	2243.0
103.90	193.0
105.90	137.0
115.80	193.0
116.90	377.0
117.80	152.0
118.80	219.0
127.90	162.0
129.90	208.0
140.80	516.0
142.90	443.0
144.90	131.0
155.00	124.0
171.90	372.0
174.00	29976.0
174.90	2313.0
175.90	28768.0
177.00	1878.0

Instrument :
MSVOA_U
ClientSampleId :
BFB38