

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072522\
 Data File : VU049866.D
 Acq On : 25 Jul 2022 14:45
 Operator : SY/MD
 Sample : VU0725WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK096

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049866.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	91	rBV	48359	55135	11.13%	1.602%
2	1.729	114	121	129	rVB2	4176	5693	1.15%	0.165%
3	1.912	169	178	196	rVB	44118	57762	11.66%	1.678%
4	2.565	369	381	399	rVB	84121	135414	27.33%	3.934%
5	3.044	519	530	545	rVB2	28381	52549	10.61%	1.526%
6	3.186	560	574	589	rVB	5057	11698	2.36%	0.340%
7	3.700	721	734	747	rVB4	10228	23042	4.65%	0.669%
8	4.639	1013	1026	1046	rBV2	61037	184054	37.15%	5.347%
9	5.063	1142	1158	1182	rBV2	82341	188677	38.08%	5.481%
10	5.726	1344	1364	1387	rBV2	165294	426674	86.12%	12.394%
11	6.250	1514	1527	1554	rBV	125461	235402	47.51%	6.838%
12	6.693	1652	1665	1687	rBV	109060	214704	43.34%	6.237%
13	7.568	1925	1937	1959	rBV	48119	84440	17.04%	2.453%
14	7.899	2027	2040	2058	rBV	178923	312845	63.14%	9.088%
15	8.182	2116	2128	2143	rBV2	28970	50497	10.19%	1.467%
16	8.639	2255	2270	2312	rBV3	204710	495440	100.00%	14.392%
17	9.420	2501	2513	2534	rBV	165838	279867	56.49%	8.130%
18	10.758	2914	2929	2948	rVB2	82538	135548	27.36%	3.938%
19	11.812	3246	3257	3273	rBV	145594	236310	47.70%	6.865%
20	12.195	3364	3376	3397	rBV	154587	256712	51.81%	7.457%




Sum of corrected areas: 3442463

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072522\
Data File : VU049866.D
Acq On : 25 Jul 2022 14:45
Operator : SY/MD
Sample : VU0725WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK096

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

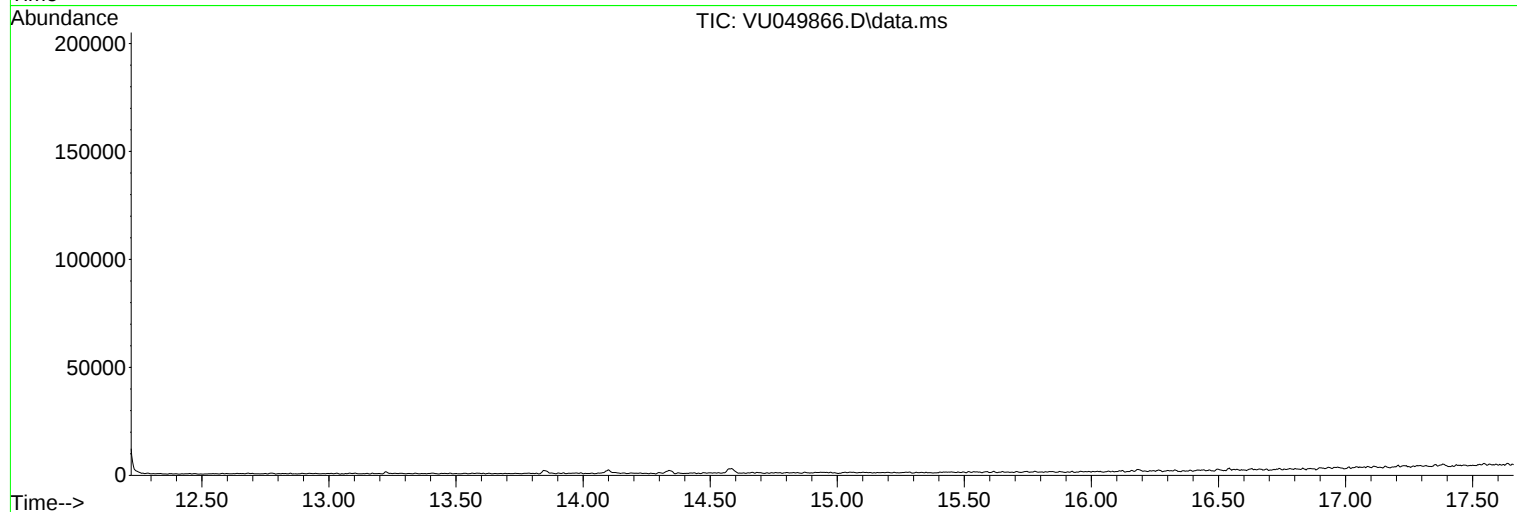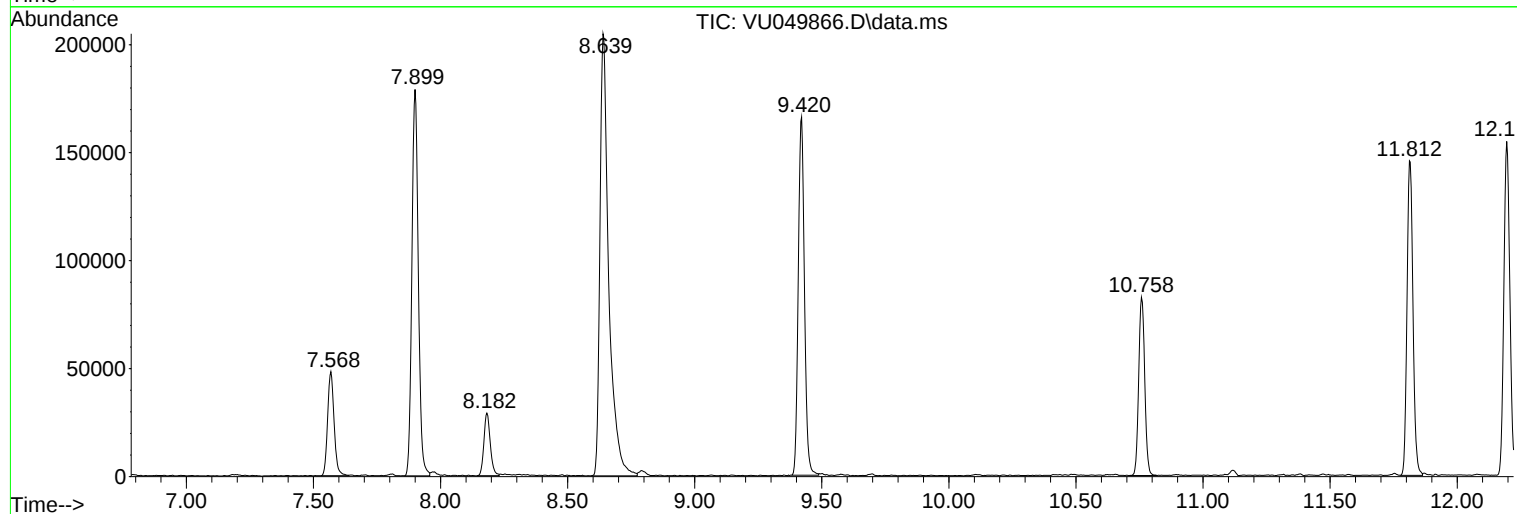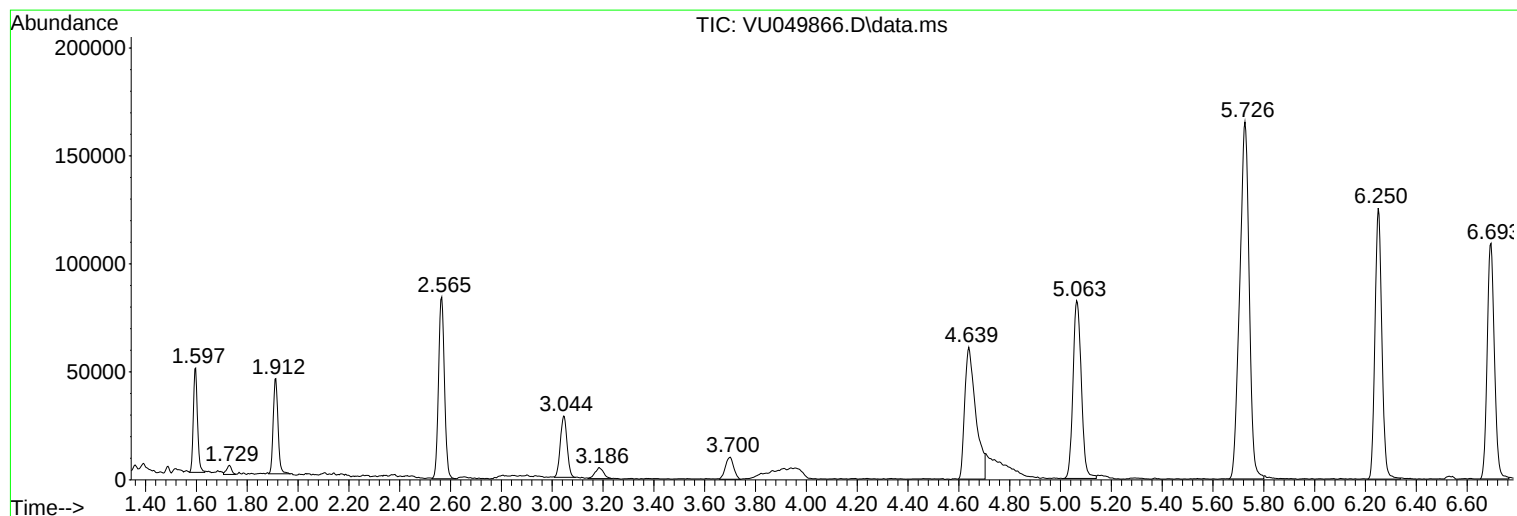

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072522\
Data File : VU049866.D
Acq On : 25 Jul 2022 14:45
Operator : SY/MD
Sample : VU0725WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK096

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072522\
Data File : VU049866.D
Acq On : 25 Jul 2022 14:45
Operator : SY/MD
Sample : VU0725WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK096

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc