

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072522\
 Data File : VU049870.D
 Acq On : 25 Jul 2022 16:28
 Operator : SY/MD
 Sample : N3802-23DL 10X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBHY6DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU049870.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.388	11	15	38	rVB3	4025	8060	1.48%	0.205%
2	1.594	72	79	92	rVB	49242	55816	10.25%	1.418%
3	1.729	114	121	127	rBV	5956	6837	1.26%	0.174%
4	1.909	169	177	191	rVB	44804	58866	10.81%	1.496%
5	2.562	366	380	396	rVB	86813	146204	26.86%	3.715%
6	3.044	517	530	545	rVB2	16803	31946	5.87%	0.812%
7	3.186	561	574	590	rVB2	8627	19676	3.61%	0.500%
8	4.652	1014	1030	1077	rBV4	86016	327994	60.25%	8.335%
9	5.064	1142	1158	1179	rBV	87786	194936	35.81%	4.954%
10	5.726	1344	1364	1382	rBV3	170560	441000	81.01%	11.207%
11	6.250	1511	1527	1550	rBV	118502	225984	41.51%	5.743%
12	6.543	1605	1618	1640	rBV	149797	285065	52.37%	7.244%
13	6.690	1651	1664	1685	rBV	112040	217321	39.92%	5.523%
14	7.568	1920	1937	1953	rBV2	49973	87436	16.06%	2.222%
15	7.899	2027	2040	2056	rBV	187067	321502	59.06%	8.170%
16	8.182	2116	2128	2143	rBV	30896	51714	9.50%	1.314%
17	8.639	2257	2270	2306	rBV2	238103	544370	100.00%	13.834%
18	9.417	2500	2512	2530	rBV	158525	269668	49.54%	6.853%
19	10.758	2917	2929	2944	rVB2	86357	139257	25.58%	3.539%
20	11.812	3245	3257	3275	rBV	141294	230573	42.36%	5.860%
21	12.195	3363	3376	3401	rVB	162432	270800	49.75%	6.882%




Sum of corrected areas: 3935025

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072522\
Data File : VU049870.D
Acq On : 25 Jul 2022 16:28
Operator : SY/MD
Sample : N3802-23DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBHY6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

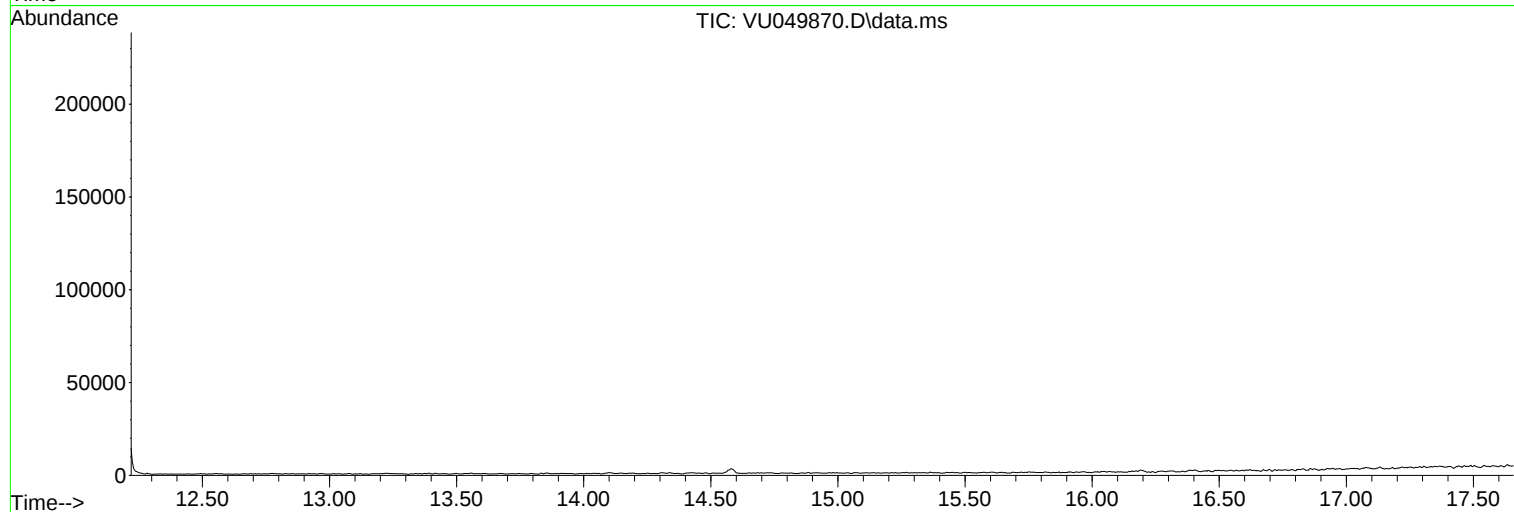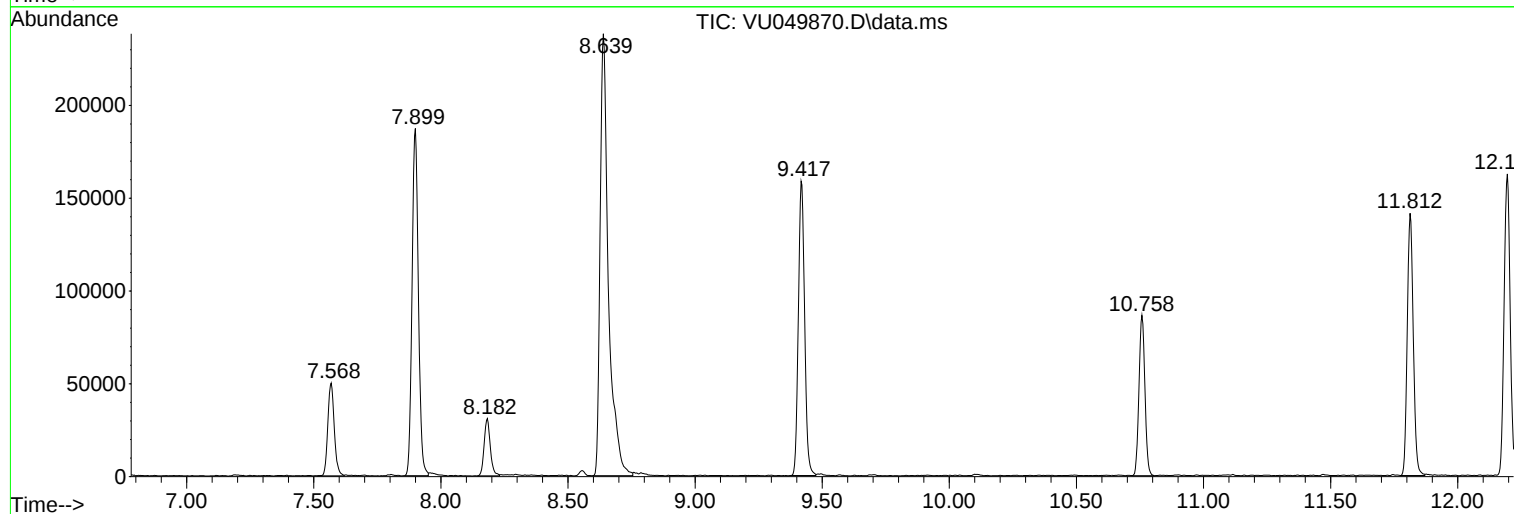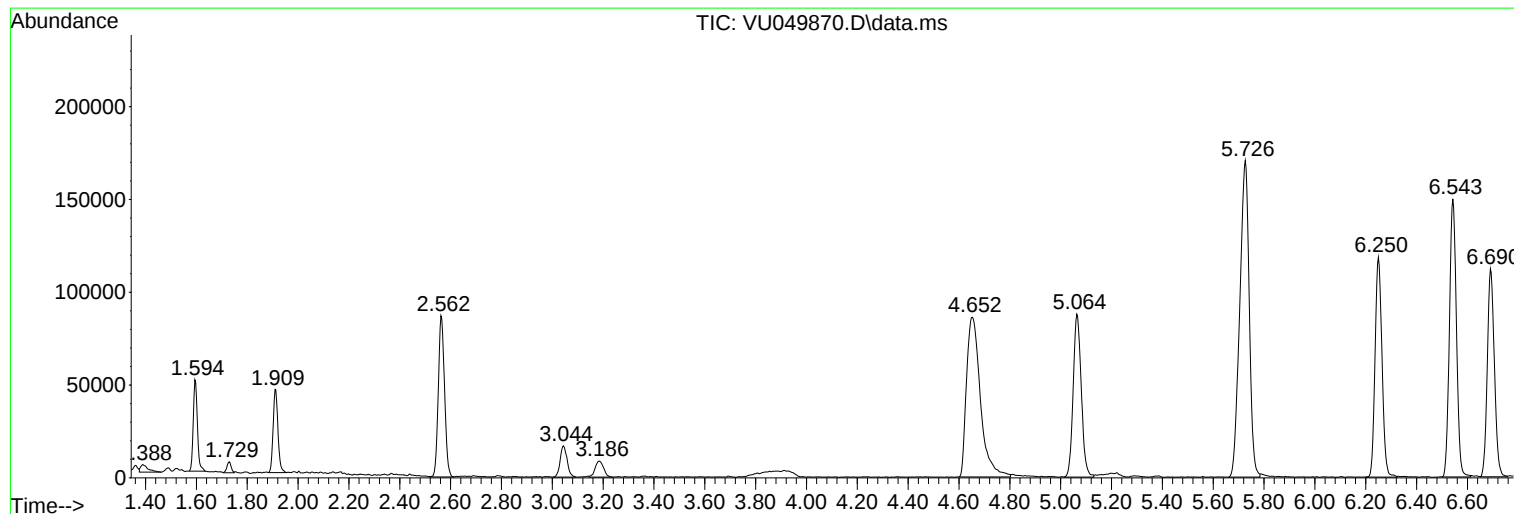

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072522\
Data File : VU049870.D
Acq On : 25 Jul 2022 16:28
Operator : SY/MD
Sample : N3802-23DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBHY6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072522\
Data File : VU049870.D
Acq On : 25 Jul 2022 16:28
Operator : SY/MD
Sample : N3802-23DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBHY6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc