

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072522\
 Data File : VU049871.D
 Acq On : 25 Jul 2022 16:51
 Operator : SY/MD
 Sample : N3802-24DL 40X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBHY7DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049871.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	90	rBV	43726	47419	9.04%	1.277%
2	1.912	169	178	186	rBV	42111	53042	10.11%	1.428%
3	1.951	186	190	198	rVB	4462	5412	1.03%	0.146%
4	2.565	369	381	393	rBV	72093	117781	22.45%	3.171%
5	3.041	519	529	542	rVB	12678	23539	4.49%	0.634%
6	3.182	562	573	591	rVB2	8129	18902	3.60%	0.509%
7	4.665	1014	1034	1088	rBV2	86906	317074	60.44%	8.537%
8	5.063	1140	1158	1177	rBV	84359	186855	35.62%	5.031%
9	5.722	1344	1363	1388	rBV2	173808	421896	80.41%	11.360%
10	6.250	1513	1527	1549	rBV	111757	210440	40.11%	5.666%
11	6.542	1602	1618	1637	rBV2	168921	322094	61.39%	8.673%
12	6.693	1650	1665	1687	rBV	107376	208175	39.68%	5.605%
13	7.568	1925	1937	1953	rBV	45907	81585	15.55%	2.197%
14	7.899	2025	2040	2057	rBV	162754	282862	53.91%	7.616%
15	8.182	2114	2128	2141	rBV	29226	48506	9.25%	1.306%
16	8.645	2260	2272	2301	rBV3	227118	524651	100.00%	14.127%
17	9.417	2500	2512	2529	rBV	145892	247443	47.16%	6.663%
18	10.758	2917	2929	2944	rBV	84884	139370	26.56%	3.753%
19	11.812	3246	3257	3273	rBV	129212	208807	39.80%	5.622%
20	12.195	3362	3376	3397	rBV	152668	248056	47.28%	6.679%




Sum of corrected areas: 3713909

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072522\
Data File : VU049871.D
Acq On : 25 Jul 2022 16:51
Operator : SY/MD
Sample : N3802-24DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBHY7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

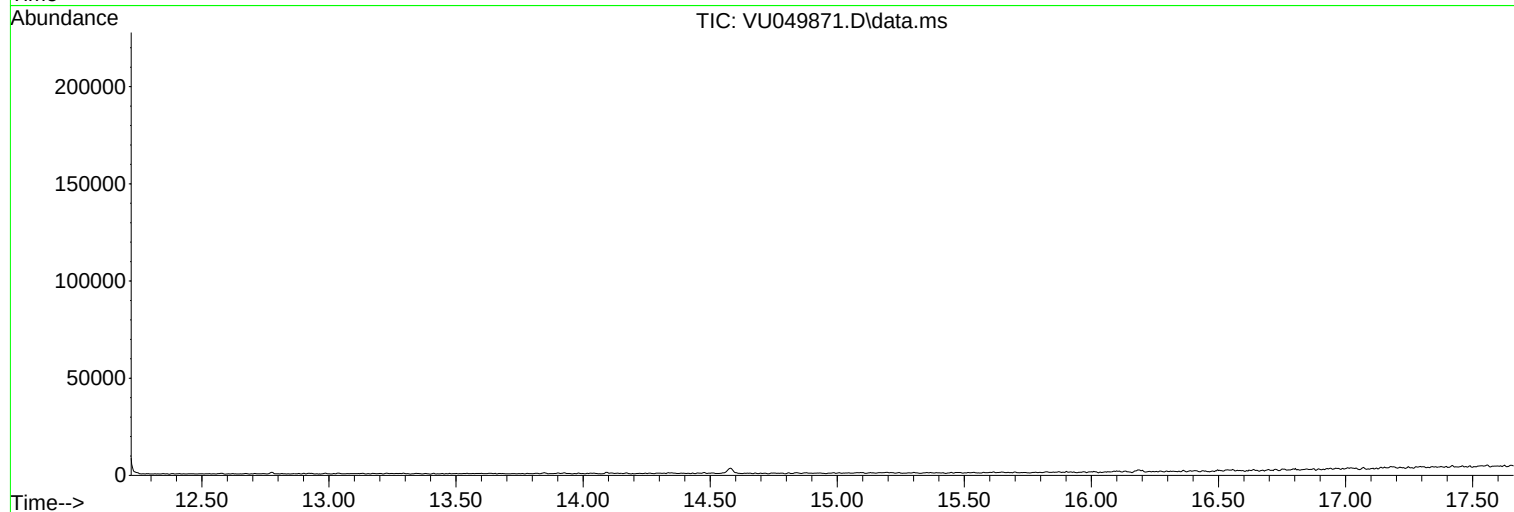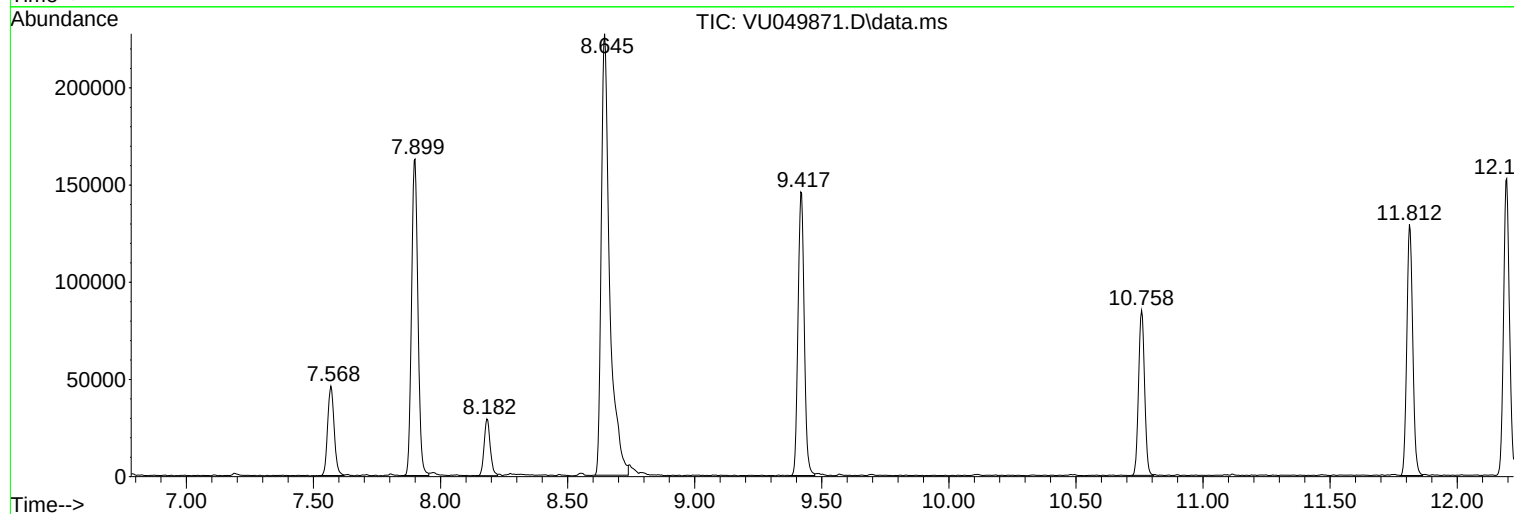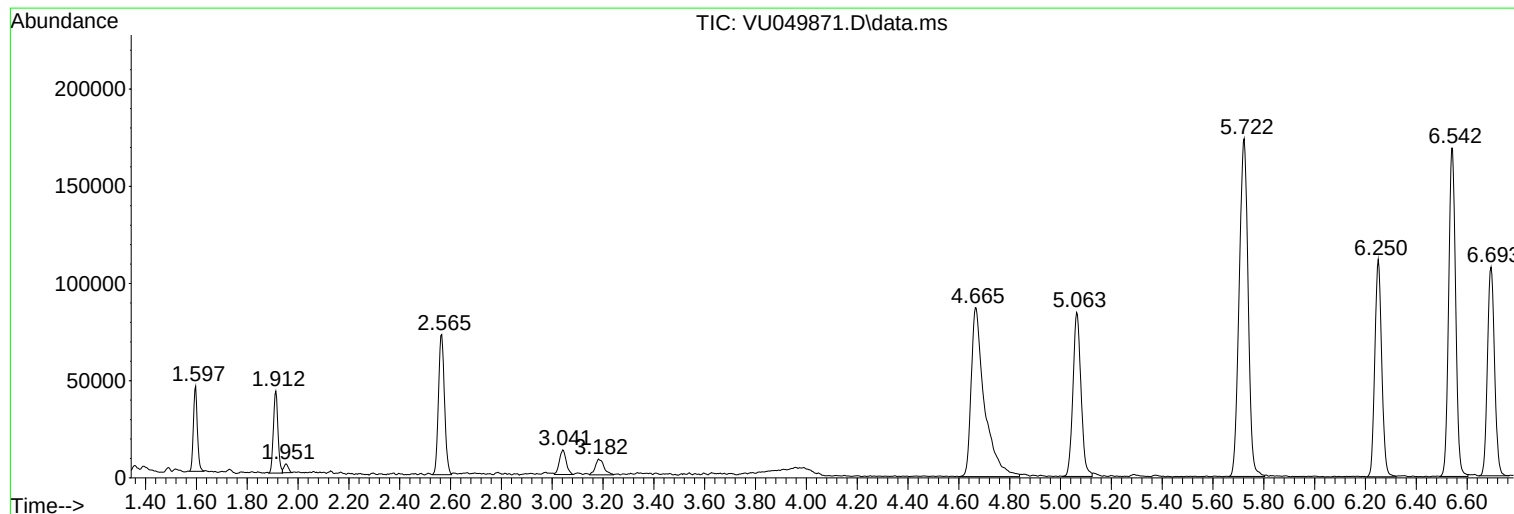

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072522\
Data File : VU049871.D
Acq On : 25 Jul 2022 16:51
Operator : SY/MD
Sample : N3802-24DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBHY7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072522\
Data File : VU049871.D
Acq On : 25 Jul 2022 16:51
Operator : SY/MD
Sample : N3802-24DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBHY7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc