

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072522\
 Data File : VU049874.D
 Acq On : 25 Jul 2022 18:05
 Operator : SY/MD
 Sample : N3802-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU049874.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.594	72	79	94	rBV	49134	55560	10.53%	1.590%
2	1.771	126	134	143	rBV	56462	66019	12.51%	1.889%
3	1.912	169	178	192	rVB	45014	59900	11.35%	1.714%
4	2.035	210	216	225	rBV	6231	7586	1.44%	0.217%
5	2.562	369	380	396	rVB	82536	132413	25.09%	3.789%
6	3.041	517	529	542	rBV	27053	47924	9.08%	1.371%
7	4.658	1018	1032	1068	rBV	65323	228157	43.24%	6.528%
8	5.063	1143	1158	1176	rBV	87495	193051	36.58%	5.524%
9	5.726	1344	1364	1382	rBV2	168918	426496	80.82%	12.204%
10	6.250	1513	1527	1543	rBV	112680	213305	40.42%	6.103%
11	6.694	1649	1665	1683	rBV	109631	211044	39.99%	6.039%
12	7.568	1924	1937	1953	rBV	48324	84110	15.94%	2.407%
13	7.899	2025	2040	2057	rBV	177419	307419	58.25%	8.796%
14	8.182	2118	2128	2140	rBV2	28474	48724	9.23%	1.394%
15	8.555	2232	2244	2253	rVB4	5312	8096	1.53%	0.232%
16	8.642	2258	2271	2298	rBV3	227250	527713	100.00%	15.100%
17	9.417	2501	2512	2532	rBV	155315	258472	48.98%	7.396%
18	10.758	2916	2929	2943	rBV	87904	139852	26.50%	4.002%
19	11.812	3246	3257	3273	rBV	132236	215185	40.78%	6.157%
20	12.195	3364	3376	3395	rBV	154108	257489	48.79%	7.368%
21	14.577	4105	4117	4129	rVB4	3336	6348	1.20%	0.182%




Sum of corrected areas: 3494863

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072522\
Data File : VU049874.D
Acq On : 25 Jul 2022 18:05
Operator : SY/MD
Sample : N3802-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

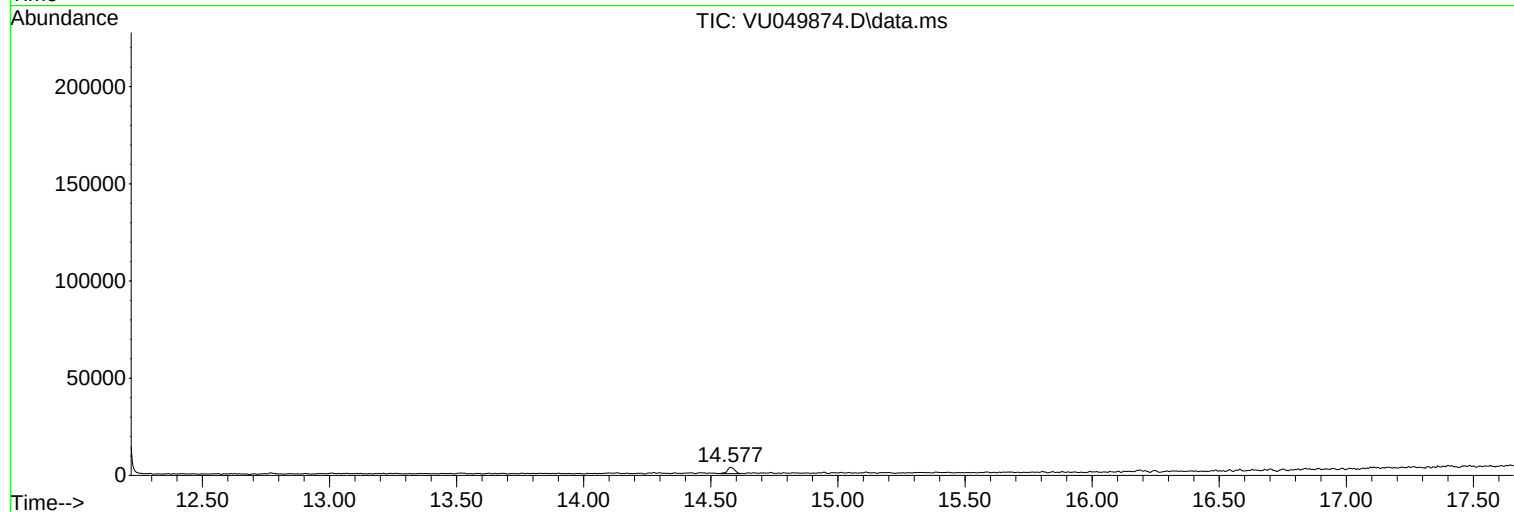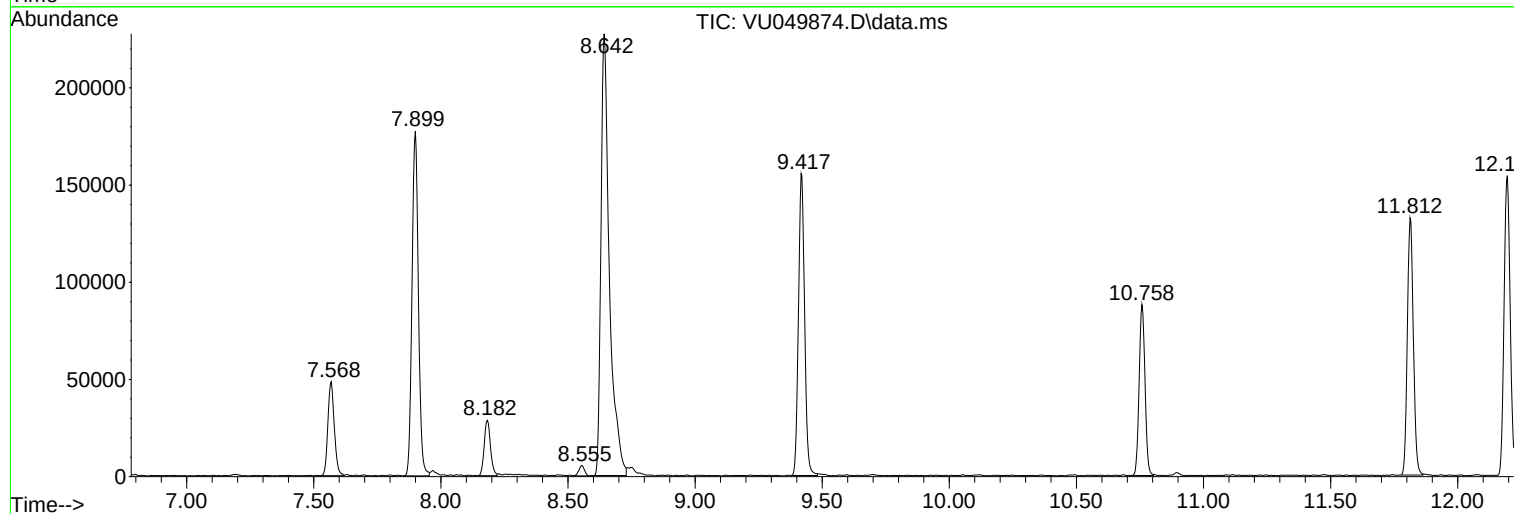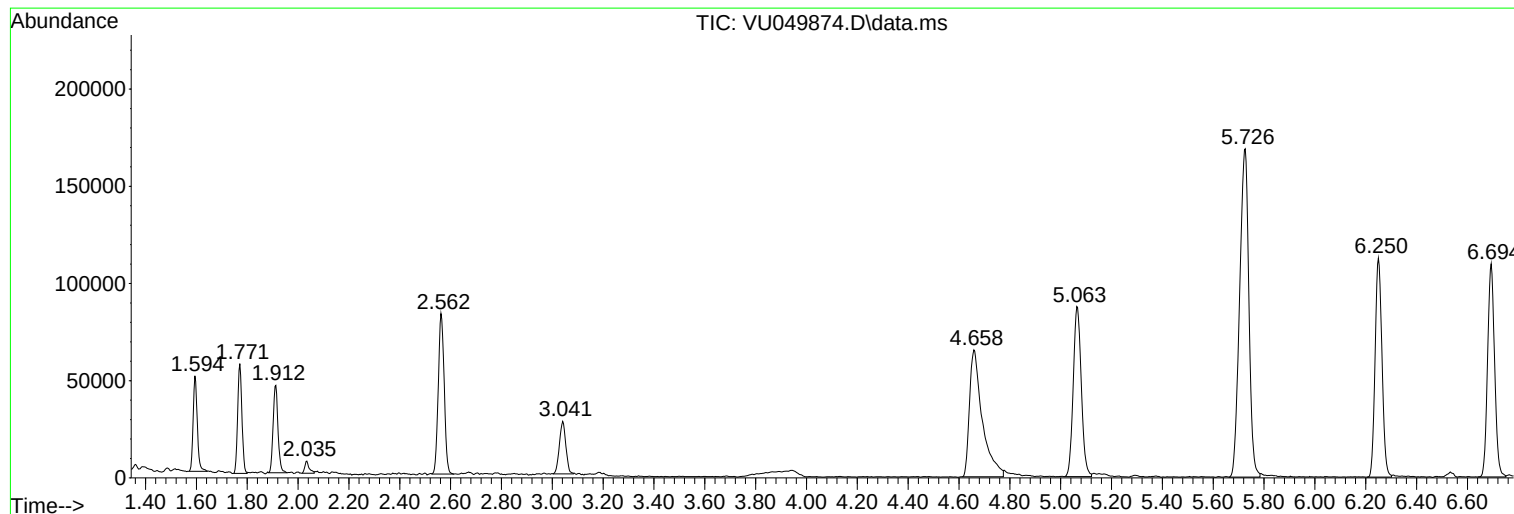

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072522\
Data File : VU049874.D
Acq On : 25 Jul 2022 18:05
Operator : SY/MD
Sample : N3802-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.771	1.55 ug/L	66019	1,4-Difluorobenzene	6.250

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			7-Octene-1,2-diol	144	C8H16O2	085866-02-0	12
2			3-Pyridinol-1-oxide	111	C5H5NO2	006602-28-4	9
3			2(1H)-Pyridinone	95	C5H5NO	000142-08-5	9
4			Bis(chloromethyl) sulfide	130	C2H4Cl2S	003592-44-7	9
5			Furan-2-carboxylic acid phenyl-(...	339	C14H8F3N3O2S	1000300-94-9	9

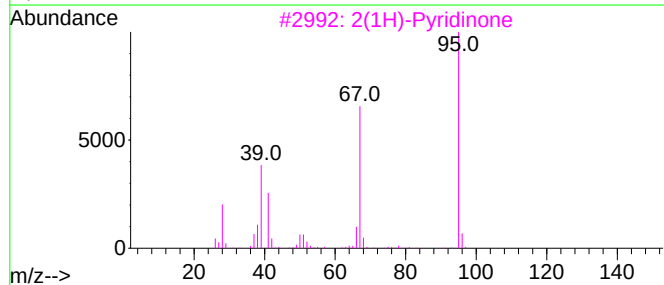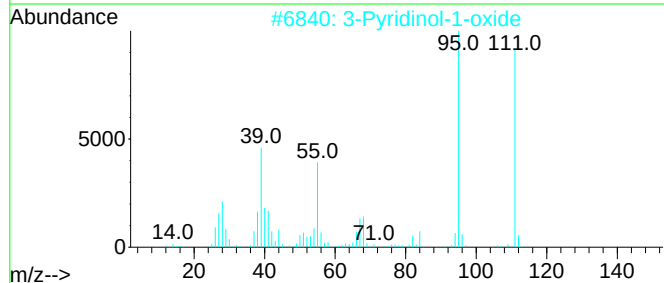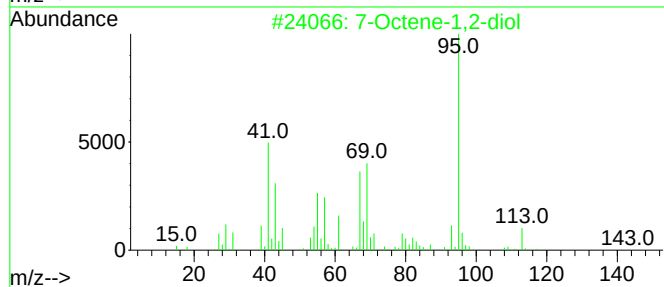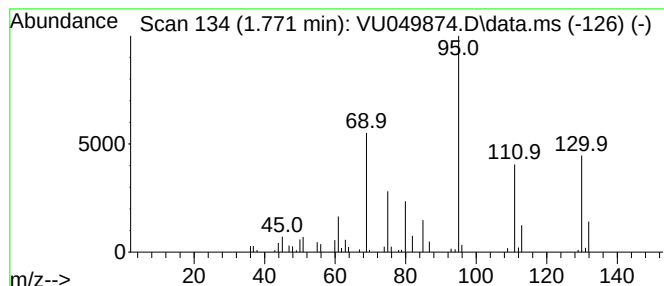

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072522\
Data File : VU049874.D
Acq On : 25 Jul 2022 18:05
Operator : SY/MD
Sample : N3802-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	1.771	1.6	ug/L	66019	1	6.250	213305	5.0