

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072522\
 Data File : VU049881.D
 Acq On : 25 Jul 2022 21:45
 Operator : SY/MD
 Sample : VU0725WBL02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK097

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049881.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.520	50	56	72	rVV4	4567	9259	1.69%	0.270%
2	1.597	72	80	94	rVV	51544	57856	10.57%	1.690%
3	1.771	128	134	141	rVB2	7977	8902	1.63%	0.260%
4	1.912	170	178	190	rVB	46047	58840	10.75%	1.719%
5	2.562	368	380	393	rBV	85862	136200	24.89%	3.978%
6	3.044	518	530	546	rVB2	12330	23067	4.22%	0.674%
7	4.645	1015	1028	1054	rBV	60436	193811	35.42%	5.661%
8	5.063	1142	1158	1176	rBV2	87115	194553	35.56%	5.682%
9	5.726	1344	1364	1384	rBV2	169054	434267	79.37%	12.684%
10	6.250	1514	1527	1550	rBV2	111563	210729	38.51%	6.155%
11	6.693	1651	1665	1683	rBV	108925	214106	39.13%	6.254%
12	7.568	1924	1937	1959	rBV2	46873	83082	15.18%	2.427%
13	7.899	2021	2040	2059	rBV	177441	312946	57.20%	9.140%
14	8.182	2116	2128	2142	rBV2	28871	49968	9.13%	1.459%
15	8.642	2255	2271	2307	rBV3	216878	547143	100.00%	15.981%
16	9.417	2500	2512	2532	rBV	153940	259349	47.40%	7.575%
17	10.758	2917	2929	2944	rBV	86611	140112	25.61%	4.092%
18	11.812	3246	3257	3279	rBV	131545	217692	39.79%	6.358%
19	12.195	3362	3376	3395	rBV	159962	265969	48.61%	7.768%
20	16.185	4602	4617	4625	rBV5	2983	5882	1.08%	0.172%




Sum of corrected areas: 3423733

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072522\
Data File : VU049881.D
Acq On : 25 Jul 2022 21:45
Operator : SY/MD
Sample : VU0725WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK097

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

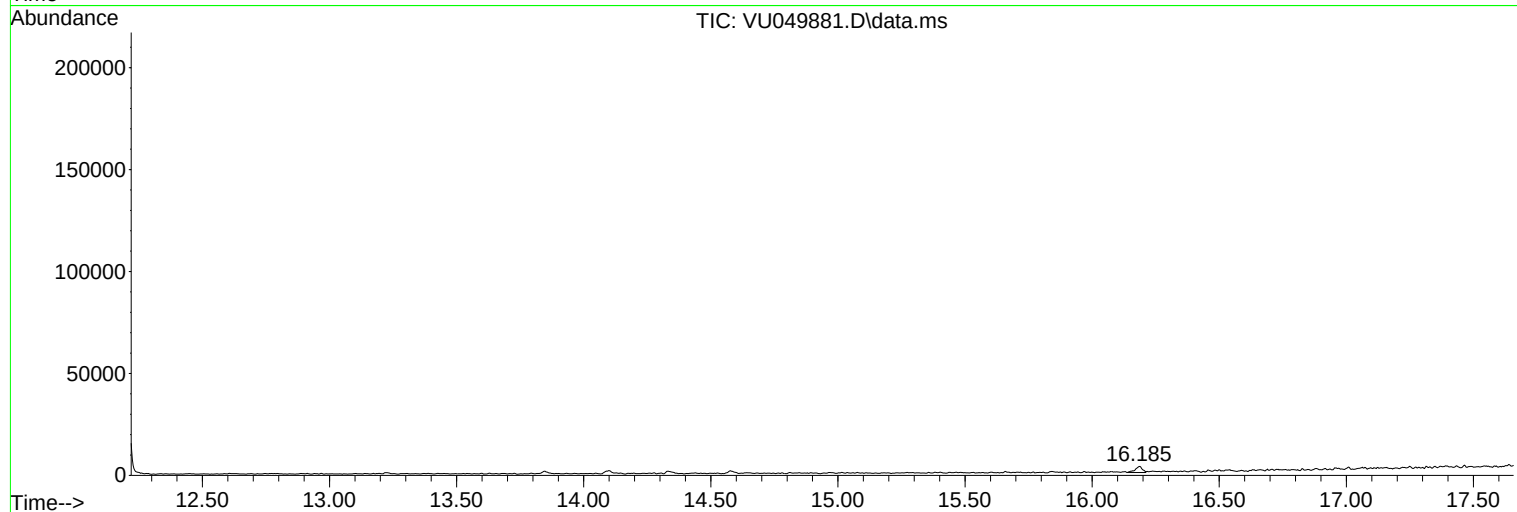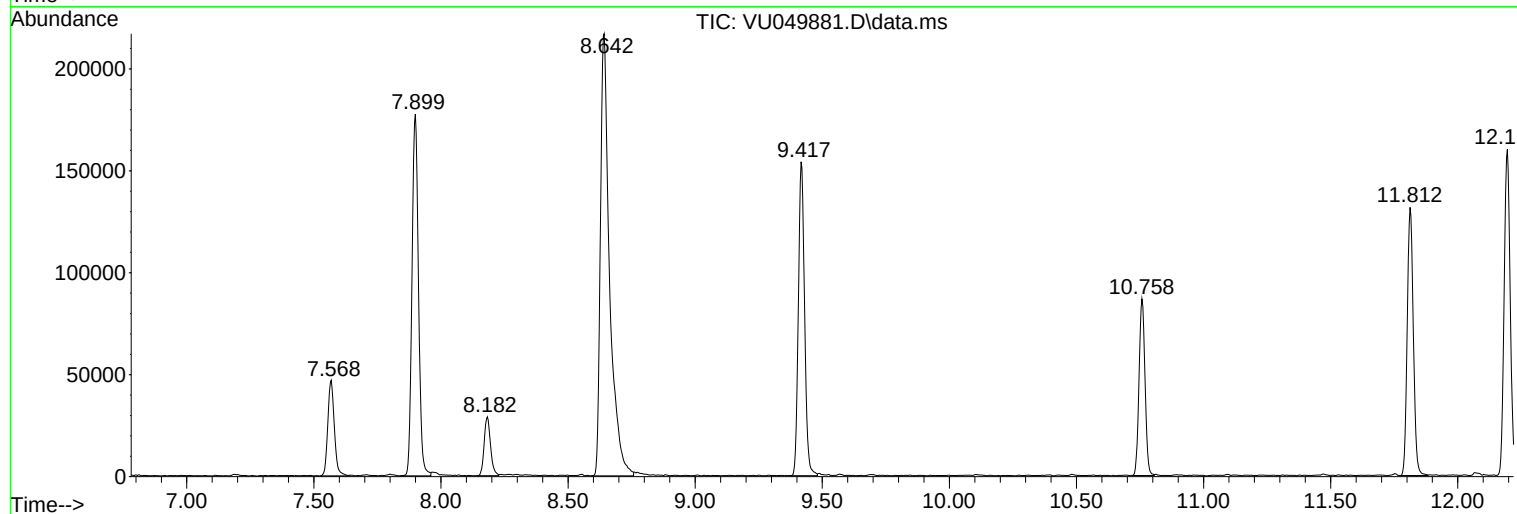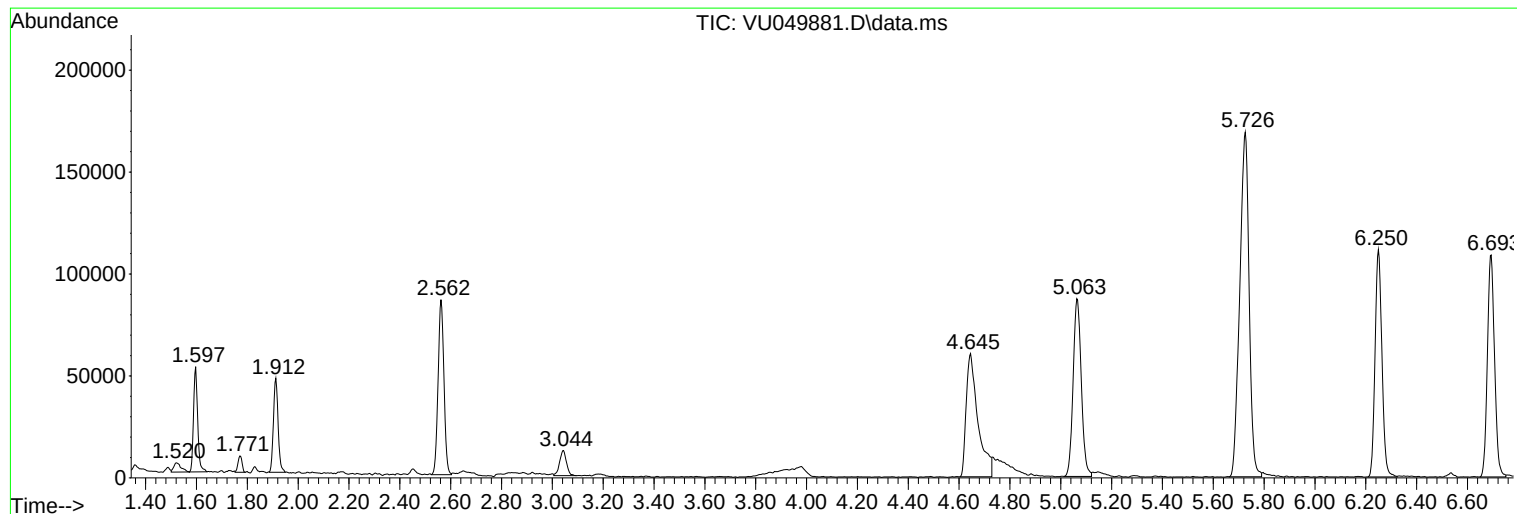

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072522\
Data File : VU049881.D
Acq On : 25 Jul 2022 21:45
Operator : SY/MD
Sample : VU0725WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK097

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072522\
Data File : VU049881.D
Acq On : 25 Jul 2022 21:45
Operator : SY/MD
Sample : VU0725WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK097

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc