
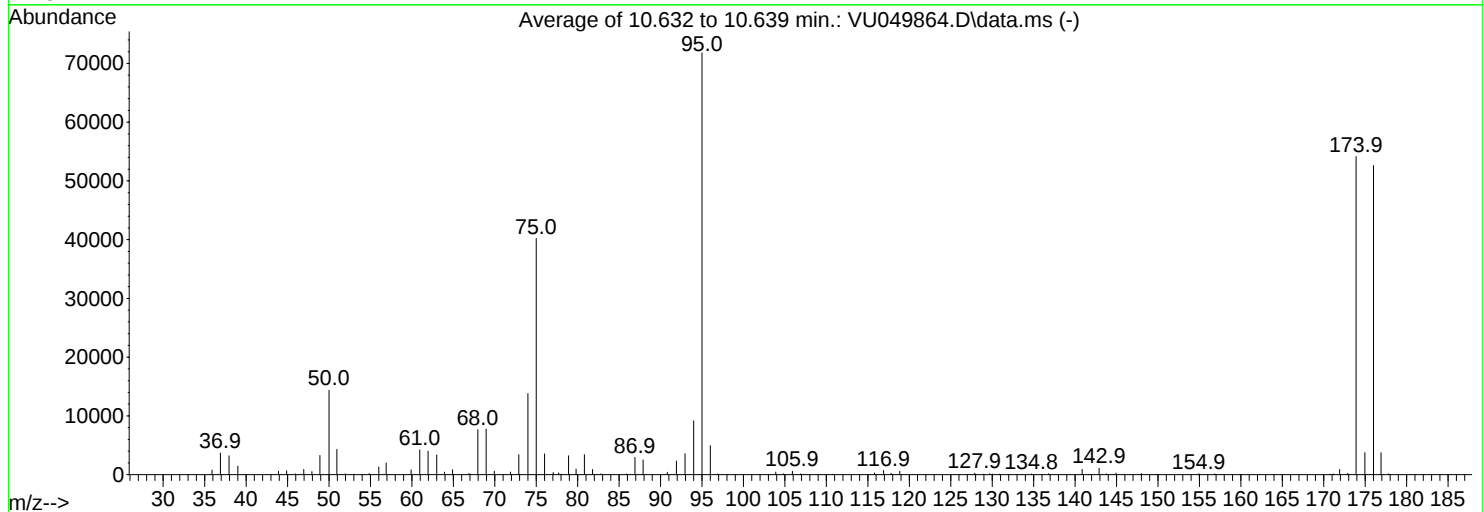


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072522\
Data File : VU049864.D
Acq On : 25 Jul 2022 09:00
Operator : SY/MD
Sample : BFB093
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB093

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Jul 27 05:17:43 2022

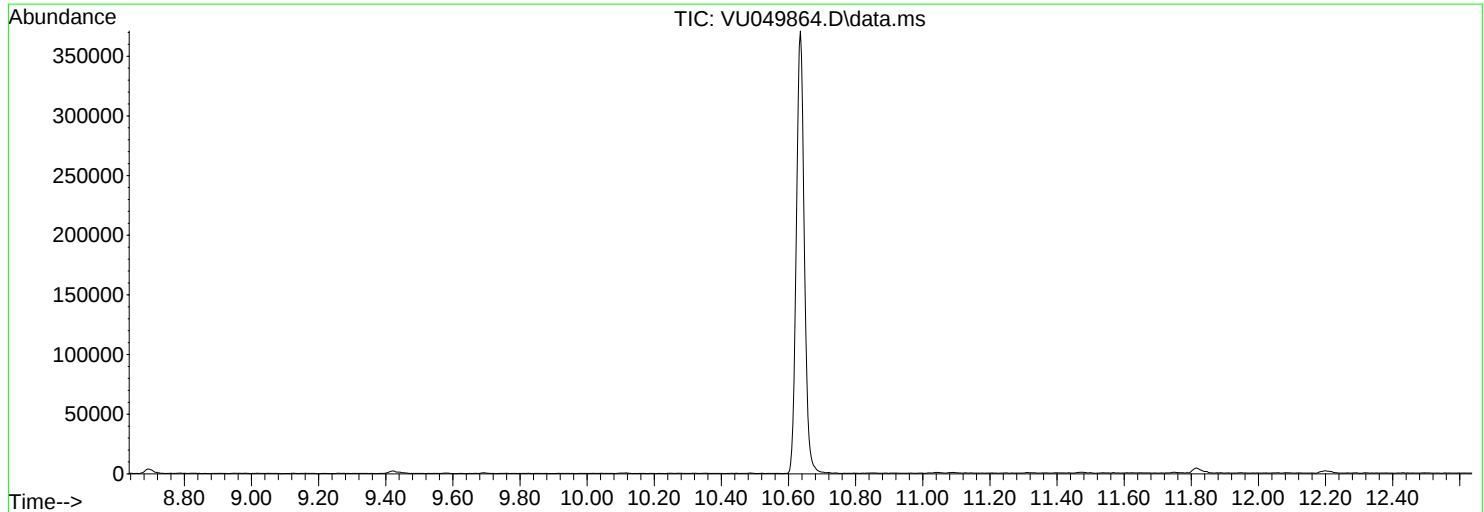

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.0	14367	PASS
75	95	30	80	56.0	40192	PASS
95	95	100	100	100.0	71805	PASS
96	95	5	9	6.9	4936	PASS
173	174	0.00	2	0.5	255	PASS
174	95	50	120	75.4	54141	PASS
175	174	5	9	7.0	3765	PASS
176	174	95	101	97.2	52637	PASS
177	176	5	9	7.1	3723	PASS

m/z	Abundance
39.90	162.0
43.90	268.0

Instrument :
MSVOA_U
ClientSampleId :
BFB093

m/z	Abundance
35.90	849.0
36.90	3824.0
37.90	3192.0
39.00	1558.0
39.90	219.0
43.90	758.0
44.90	695.0
45.90	138.0
46.90	922.0
48.00	508.0
48.90	3309.0
50.00	14497.0
50.90	4533.0
52.00	174.0
53.00	145.0
54.90	177.0
56.00	1355.0
56.90	2018.0
59.90	832.0
61.00	4289.0
61.90	4067.0
63.00	3423.0
64.00	531.0
64.90	746.0
66.90	223.0
67.90	7717.0
68.90	8123.0
70.00	673.0
71.90	489.0
72.90	3375.0
74.00	13973.0
75.00	40112.0
76.00	3628.0
77.00	337.0
77.80	280.0
78.90	3397.0
79.80	1009.0
80.80	3266.0
81.80	861.0
82.80	135.0
85.90	187.0
86.90	2817.0
87.90	2466.0
90.80	457.0
91.90	2359.0
92.90	3490.0
94.00	9080.0
95.00	71256.0
96.00	4962.0
96.90	157.0
103.90	413.0
104.80	218.0
105.90	557.0
106.90	144.0
115.80	322.0
116.90	747.0
117.70	236.0
118.90	554.0
127.90	264.0
128.90	101.0
129.80	195.0
134.70	115.0
136.80	208.0
140.80	795.0
141.60	123.0
142.90	1080.0
143.80	133.0
144.90	318.0
148.00	184.0
154.90	164.0
156.80	127.0
170.70	154.0
171.90	863.0
173.90	53312.0
174.90	3899.0
176.00	51408.0
176.90	3881.0
177.90	104.0

Instrument :
MSVOA_U
ClientSampleId :
BFB093

m/z	Abundance
35.90	842.0
36.90	3743.0
37.90	3297.0
39.00	1460.0
40.00	229.0
43.90	822.0
44.90	653.0
46.00	139.0
47.00	923.0
48.00	553.0
48.90	3377.0
50.00	14761.0
50.90	4380.0
52.00	179.0
53.00	107.0
54.80	174.0
56.00	1345.0
56.90	1989.0
57.90	100.0
59.90	824.0
61.00	4384.0
61.90	4128.0
63.00	3471.0
64.00	431.0
64.90	870.0
66.90	210.0
68.00	7835.0
68.90	8053.0
70.00	639.0
71.90	459.0
72.90	3478.0
74.00	14200.0
75.00	41664.0
76.00	3627.0
77.10	360.0
77.70	272.0
78.00	265.0
78.90	3289.0
79.80	947.0
80.80	3548.0
81.80	845.0
82.80	146.0
85.90	161.0
86.90	2975.0
87.90	2544.0
90.80	423.0
91.90	2384.0
93.00	3730.0
94.00	9394.0
95.00	74144.0
96.00	5151.0
96.90	155.0
103.90	437.0
104.80	184.0
105.90	618.0
106.90	125.0
110.80	111.0
115.80	312.0
116.90	714.0
117.80	246.0
118.90	584.0
127.90	268.0
128.90	119.0
129.70	171.0
130.00	164.0
130.90	125.0
134.80	150.0
136.80	178.0
140.90	954.0
142.90	1110.0
143.80	139.0
144.90	260.0
146.00	114.0
148.00	210.0
149.70	111.0
154.90	188.0
156.80	150.0
170.80	135.0
171.10	144.0
171.90	901.0
173.90	55944.0
175.00	3824.0
176.00	54376.0
176.90	3823.0
177.80	133.0

Instrument :
MSVOA_U
ClientSampleId :
BFB093

m/z	Abundance
35.90	706.0
36.90	3436.0
38.00	3159.0
39.00	1302.0
40.00	217.0
43.90	917.0
44.90	623.0
46.00	136.0
47.00	807.0
47.90	528.0
48.90	3091.0
50.00	13843.0
51.00	4002.0
51.90	150.0
54.80	215.0
56.00	1224.0
56.90	1924.0
59.90	774.0
60.90	4007.0
62.00	3839.0
63.00	3178.0
63.90	377.0
64.90	922.0
66.90	221.0
68.00	7382.0
69.00	7154.0
69.90	516.0
71.90	399.0
72.90	3338.0
74.00	13235.0
75.00	38800.0
76.00	3365.0
77.10	346.0
77.60	322.0
78.90	2965.0
79.80	935.0
80.80	3419.0
81.80	885.0
82.80	133.0
85.90	102.0
86.90	3011.0
87.90	2492.0
90.80	353.0
91.90	2201.0
92.90	3503.0
94.00	9004.0
95.00	70016.0
96.00	4695.0
96.90	122.0
103.90	455.0
104.80	128.0
105.90	549.0
106.90	112.0
110.80	112.0
115.80	289.0
116.90	633.0
117.90	277.0
118.80	560.0
127.90	229.0
128.90	148.0
129.60	147.0
130.10	135.0
130.90	134.0
134.80	178.0
136.80	140.0
140.90	922.0
141.90	125.0
142.90	1071.0
143.80	126.0
145.00	208.0
145.90	120.0
148.00	219.0
155.00	184.0
156.90	148.0
171.20	199.0
171.90	815.0
172.90	766.0
173.90	53168.0
175.00	3571.0
176.00	52128.0
176.90	3465.0
177.80	134.0

Instrument :
MSVOA_U
ClientSampleId :
BFB093