


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072618\
 Data File : VU025641.D
 Acq On : 26 Jul 2018 09:05
 Operator : MD/SY
 Sample : BFB50
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB50

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis
 Last Update : Mon Aug 06 01:30:36 2018

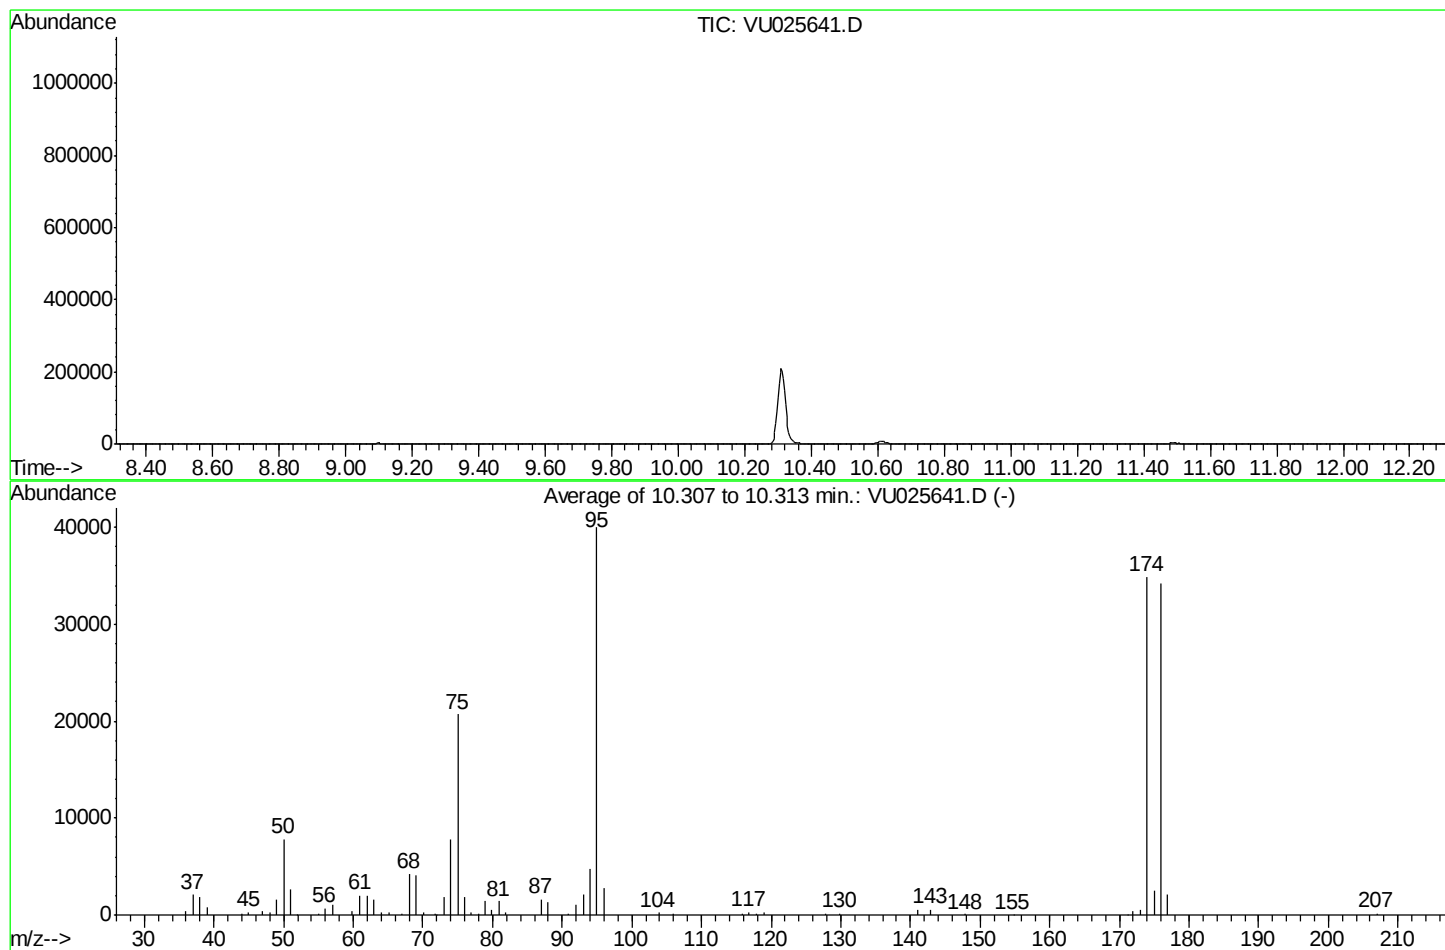

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	7827	PASS
75	95	30	80	51.7	20690	PASS
95	95	100	100	100.0	39997	PASS
96	95	5	9	6.9	2770	PASS
173	174	0.00	2	1.4	473	PASS
174	95	50	120	87.3	34917	PASS
175	174	5	9	7.1	2467	PASS
176	174	95	101	97.8	34154	PASS
177	176	5	9	6.2	2134	PASS

m/z	Abundance
39.80	147.0
43.90	432.0

Instrument :
MSVOA_U
ClientSampleId :
BFB50

m/z	Abundance
36.00	353.0
37.00	2213.0
38.00	1883.0
39.00	779.0
40.00	132.0
44.00	582.0
45.00	292.0
46.90	380.0
48.00	294.0
49.00	1642.0
50.00	7698.0
51.00	2499.0
51.90	105.0
55.90	725.0
57.00	1068.0
59.90	446.0
61.00	1946.0
62.00	2093.0
63.00	1529.0
63.90	251.0
65.10	293.0
67.00	166.0
68.00	4367.0
69.00	3888.0
70.10	333.0
71.80	224.0
73.00	1812.0
74.00	7530.0
75.00	20352.0
76.00	1783.0
76.90	247.0
78.00	140.0
78.90	1411.0
79.90	494.0
80.90	1321.0
81.90	300.0
87.00	1457.0
88.00	1295.0
90.80	208.0
92.00	1055.0
93.00	2039.0
94.00	4859.0
95.00	39144.0
96.00	2804.0
103.90	221.0
105.80	154.0
115.90	196.0
116.80	363.0
117.80	102.0
119.00	230.0
127.90	206.0
129.90	227.0
141.00	509.0
142.90	506.0
154.80	104.0
171.90	319.0
172.90	453.0
174.00	32944.0
174.90	2389.0
176.00	32048.0
176.90	2080.0
207.00	156.0

Instrument :
MSVOA_U
ClientSampleId :
BFB50

m/z	Abundance
36.00	364.0
37.00	2143.0
38.00	1887.0
39.00	838.0
40.00	113.0
44.00	550.0
45.00	347.0
47.00	434.0
48.00	331.0
49.10	1617.0
50.00	8145.0
51.00	2726.0
55.00	132.0
55.90	743.0
57.00	1163.0
59.90	387.0
61.00	2058.0
62.00	2124.0
63.00	1586.0
64.00	304.0
65.00	281.0
66.90	186.0
68.00	4356.0
69.00	4255.0
70.00	273.0
71.80	241.0
73.00	1903.0
74.00	8282.0
75.00	21416.0
76.00	1870.0
76.90	252.0
78.00	204.0
78.90	1451.0
79.90	515.0
80.90	1481.0
81.90	300.0
87.00	1678.0
88.00	1428.0
90.90	212.0
92.00	1161.0
93.00	2190.0
94.00	4911.0
95.00	41344.0
96.00	2813.0
103.80	255.0
105.80	162.0
116.00	195.0
116.80	333.0
117.80	121.0
118.90	237.0
127.90	187.0
129.90	206.0
141.00	543.0
142.90	561.0
147.90	103.0
171.80	399.0
173.00	491.0
174.00	36072.0
175.00	2534.0
176.00	35056.0
176.90	2124.0
207.00	192.0

Instrument :
MSVOA_U
ClientSampleId :
BFB50

m/z	Abundance
36.00	356.0
37.00	1831.0
38.00	1675.0
39.00	746.0
44.00	542.0
45.00	364.0
47.00	446.0
48.00	329.0
49.00	1602.0
50.00	7640.0
51.00	2529.0
55.10	161.0
56.00	704.0
57.00	1119.0
59.90	325.0
61.00	2096.0
62.00	1856.0
63.00	1481.0
64.00	282.0
65.00	286.0
66.90	160.0
68.00	4142.0
69.00	4248.0
70.00	252.0
72.00	210.0
73.00	1848.0
74.00	7664.0
75.00	20304.0
76.00	1737.0
76.90	239.0
78.00	205.0
78.90	1339.0
79.90	450.0
80.90	1500.0
81.90	260.0
87.00	1689.0
88.00	1387.0
90.90	164.0
92.00	1149.0
93.00	2026.0
94.00	4575.0
95.00	39504.0
96.00	2693.0
103.80	209.0
105.90	155.0
116.00	185.0
116.80	264.0
117.80	133.0
118.80	251.0
127.80	189.0
129.90	156.0
141.00	550.0
142.90	553.0
147.90	121.0
171.10	124.0
171.90	417.0
172.90	475.0
174.00	35736.0
175.00	2480.0
176.00	35360.0
176.90	2198.0
206.90	205.0

Instrument :
MSVOA_U
ClientSampleId :
BFB50