

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU072619\
 Data File : VU033455.D
 Acq On : 26 Jul 2019 15:56
 Operator : JC/SP
 Sample : K3976-17DL 4X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CC5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.177	23	27	33	rBV3	2272	2311	0.23%	0.028%
2	1.389	86	93	108	rVB	148677	154048	15.62%	1.842%
3	1.547	134	142	149	rVB	25323	31922	3.24%	0.382%
4	1.669	172	180	195	rVB	123968	159786	16.20%	1.911%
5	1.878	238	245	252	rBV7	3087	4319	0.44%	0.052%
6	2.254	352	362	375	rVB	226293	345969	35.08%	4.138%
7	2.434	408	418	430	rBV3	3377	7090	0.72%	0.085%
8	2.524	442	446	449	rBV	249	248	0.03%	0.003%
9	2.547	450	453	456	rVV2	548	342	0.03%	0.004%
10	2.569	457	460	462	rVV2	443	307	0.03%	0.004%
11	2.595	466	468	471	rBV	419	276	0.03%	0.003%
12	2.682	489	495	501	rVB4	986	1380	0.14%	0.017%
13	2.820	525	538	553	rVB	8487	18020	1.83%	0.216%
14	3.129	629	634	639	rBV2	247	312	0.03%	0.004%
15	3.183	647	651	656	rVB3	201	229	0.02%	0.003%
16	3.350	699	703	707	rBV2	324	325	0.03%	0.004%
17	3.415	720	723	727	rVB2	214	201	0.02%	0.002%
18	3.473	734	741	743	rBV2	169	191	0.02%	0.002%
19	3.531	756	759	764	rVB	292	223	0.02%	0.003%
20	3.559	764	768	771	rBV2	296	220	0.02%	0.003%
21	3.601	777	781	785	rBV2	353	230	0.02%	0.003%
22	3.945	884	888	892	rBV2	383	357	0.04%	0.004%
23	4.016	907	910	913	rVB	281	205	0.02%	0.002%
24	4.077	925	929	930	rBV	308	183	0.02%	0.002%
25	4.151	938	952	988	rBV	94231	272080	27.59%	3.254%
26	4.621	1081	1098	1122	rBV	170480	418673	42.45%	5.007%
27	4.759	1137	1141	1142	rBV3	444	285	0.03%	0.003%
28	4.810	1154	1157	1161	rVB2	418	264	0.03%	0.003%
29	4.855	1167	1171	1173	rBV2	743	638	0.06%	0.008%
30	4.910	1184	1188	1191	rVB	305	209	0.02%	0.002%
31	4.961	1201	1204	1208	rVV2	575	448	0.05%	0.005%
32	5.109	1233	1250	1272	rBV	173071	398210	40.38%	4.762%
33	5.228	1284	1287	1290	rVB3	319	210	0.02%	0.003%
34	5.315	1290	1314	1352	rBV2	322671	986234	100.00%	11.795%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU072619\
 Data File : VU033455.D
 Acq On : 26 Jul 2019 15:56
 Operator : JC/SP
 Sample : K3976-17DL 4X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CC5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071219WMA.M
 Title : VOC Analysis

35	5.485	1364	1367	1370	rBV2	766	397	0.04%	0.005%
36	5.614	1404	1407	1411	rBV3	187	177	0.02%	0.002%
37	5.640	1411	1415	1416	rBV2	347	240	0.02%	0.003%
38	5.730	1441	1443	1446	rVB2	386	198	0.02%	0.002%
39	5.765	1451	1454	1460	rBV2	455	370	0.04%	0.004%
40	5.865	1468	1485	1528	rBV	301115	611853	62.04%	7.317%
41	6.167	1565	1579	1593	rBV2	48332	96018	9.74%	1.148%
42	6.309	1609	1623	1645	rBV	226822	451730	45.80%	5.402%
43	6.421	1655	1658	1660	rBV2	433	322	0.03%	0.004%
44	6.473	1669	1674	1678	rBV2	367	427	0.04%	0.005%
45	6.575	1702	1706	1709	rVB	240	213	0.02%	0.003%
46	6.682	1735	1739	1742	rBV	231	223	0.02%	0.003%
47	6.739	1752	1757	1765	rVB2	291	453	0.05%	0.005%
48	6.778	1765	1769	1773	rBV	227	246	0.02%	0.003%
49	7.000	1831	1838	1840	rBV2	200	248	0.03%	0.003%
50	7.048	1850	1853	1857	rBV	254	262	0.03%	0.003%
51	7.109	1868	1872	1876	rVB2	252	217	0.02%	0.003%
52	7.209	1890	1903	1921	rBV	120190	213363	21.63%	2.552%
53	7.546	1992	2008	2048	rBV	410319	745231	75.56%	8.912%
54	7.833	2082	2097	2120	rBV2	84818	149139	15.12%	1.784%
55	7.974	2138	2141	2144	rVB2	432	274	0.03%	0.003%
56	8.164	2192	2200	2206	rBV4	1730	2783	0.28%	0.033%
57	8.209	2206	2214	2229	rVB3	14856	25189	2.55%	0.301%
58	8.296	2229	2241	2277	rBV	274898	511154	51.83%	6.113%
59	8.572	2323	2327	2330	rBV3	315	227	0.02%	0.003%
60	8.752	2380	2383	2388	rVB3	336	263	0.03%	0.003%
61	8.884	2419	2424	2426	rBV2	416	396	0.04%	0.005%
62	8.932	2434	2439	2441	rBV2	222	214	0.02%	0.003%
63	8.974	2448	2452	2455	rBV	298	240	0.02%	0.003%
64	9.074	2470	2483	2524	rBV	456686	790312	80.13%	9.452%
65	9.286	2546	2549	2553	rVV3	304	260	0.03%	0.003%
66	9.318	2556	2559	2563	rVB	216	181	0.02%	0.002%
67	9.341	2563	2566	2571	rBV	231	232	0.02%	0.003%
68	9.534	2623	2626	2630	rVB2	306	237	0.02%	0.003%
69	9.566	2630	2636	2639	rBV2	263	285	0.03%	0.003%
70	9.585	2639	2642	2645	rBV	246	177	0.02%	0.002%
71	9.881	2731	2734	2736	rBV	299	179	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU072619\
 Data File : VU033455.D
 Acq On : 26 Jul 2019 15:56
 Operator : JC/SP
 Sample : K3976-17DL 4X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CC5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071219WMA.M
 Title : VOC Analysis

72	10.003	2767	2772	2774	rBV2	200	186	0.02%	0.002%
73	10.090	2794	2799	2806	rVB3	411	649	0.07%	0.008%
74	10.225	2838	2841	2848	rVB2	377	389	0.04%	0.005%
75	10.302	2860	2865	2868	rBV	392	371	0.04%	0.004%
76	10.321	2868	2871	2875	rVB2	285	239	0.02%	0.003%
77	10.360	2880	2883	2887	rVB2	363	341	0.03%	0.004%
78	10.415	2887	2900	2924	rBV	350849	559937	56.78%	6.696%
79	10.591	2951	2955	2966	rVB5	1631	2188	0.22%	0.026%
80	10.701	2984	2989	2991	rBV2	401	406	0.04%	0.005%
81	10.797	3017	3019	3023	rVB2	239	177	0.02%	0.002%
82	10.833	3023	3030	3034	rBV2	267	357	0.04%	0.004%
83	10.916	3054	3056	3061	rVB	315	203	0.02%	0.002%
84	11.228	3151	3153	3159	rBV3	277	248	0.03%	0.003%
85	11.469	3215	3228	3248	rBV	424777	683387	69.29%	8.173%
86	11.588	3261	3265	3268	rBV4	598	497	0.05%	0.006%
87	11.665	3286	3289	3293	rVB2	718	453	0.05%	0.005%
88	11.701	3296	3300	3303	rBV3	548	340	0.03%	0.004%
89	11.752	3310	3316	3319	rBV5	438	410	0.04%	0.005%
90	11.845	3332	3345	3374	rBV	428647	696950	70.67%	8.335%
91	12.074	3413	3416	3424	rVB5	528	562	0.06%	0.007%
92	12.144	3435	3438	3443	rVV3	557	430	0.04%	0.005%
93	12.270	3472	3477	3480	rBV3	388	410	0.04%	0.005%
94	12.575	3568	3572	3575	rBV2	408	285	0.03%	0.003%
95	12.627	3585	3588	3592	rVB2	360	240	0.02%	0.003%
96	12.855	3655	3659	3662	rBV3	256	267	0.03%	0.003%
97	12.990	3698	3701	3706	rBV3	516	334	0.03%	0.004%
98	13.373	3816	3820	3826	rBV3	390	522	0.05%	0.006%
99	15.186	4380	4384	4386	rBV2	516	457	0.05%	0.005%
100	15.311	4420	4423	4428	rBV4	661	641	0.06%	0.008%


Sum of corrected areas: 8361751

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU072619\
Data File : VU033455.D
Acq On : 26 Jul 2019 15:56
Operator : JC/SP
Sample : K3976-17DL 4X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CC5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

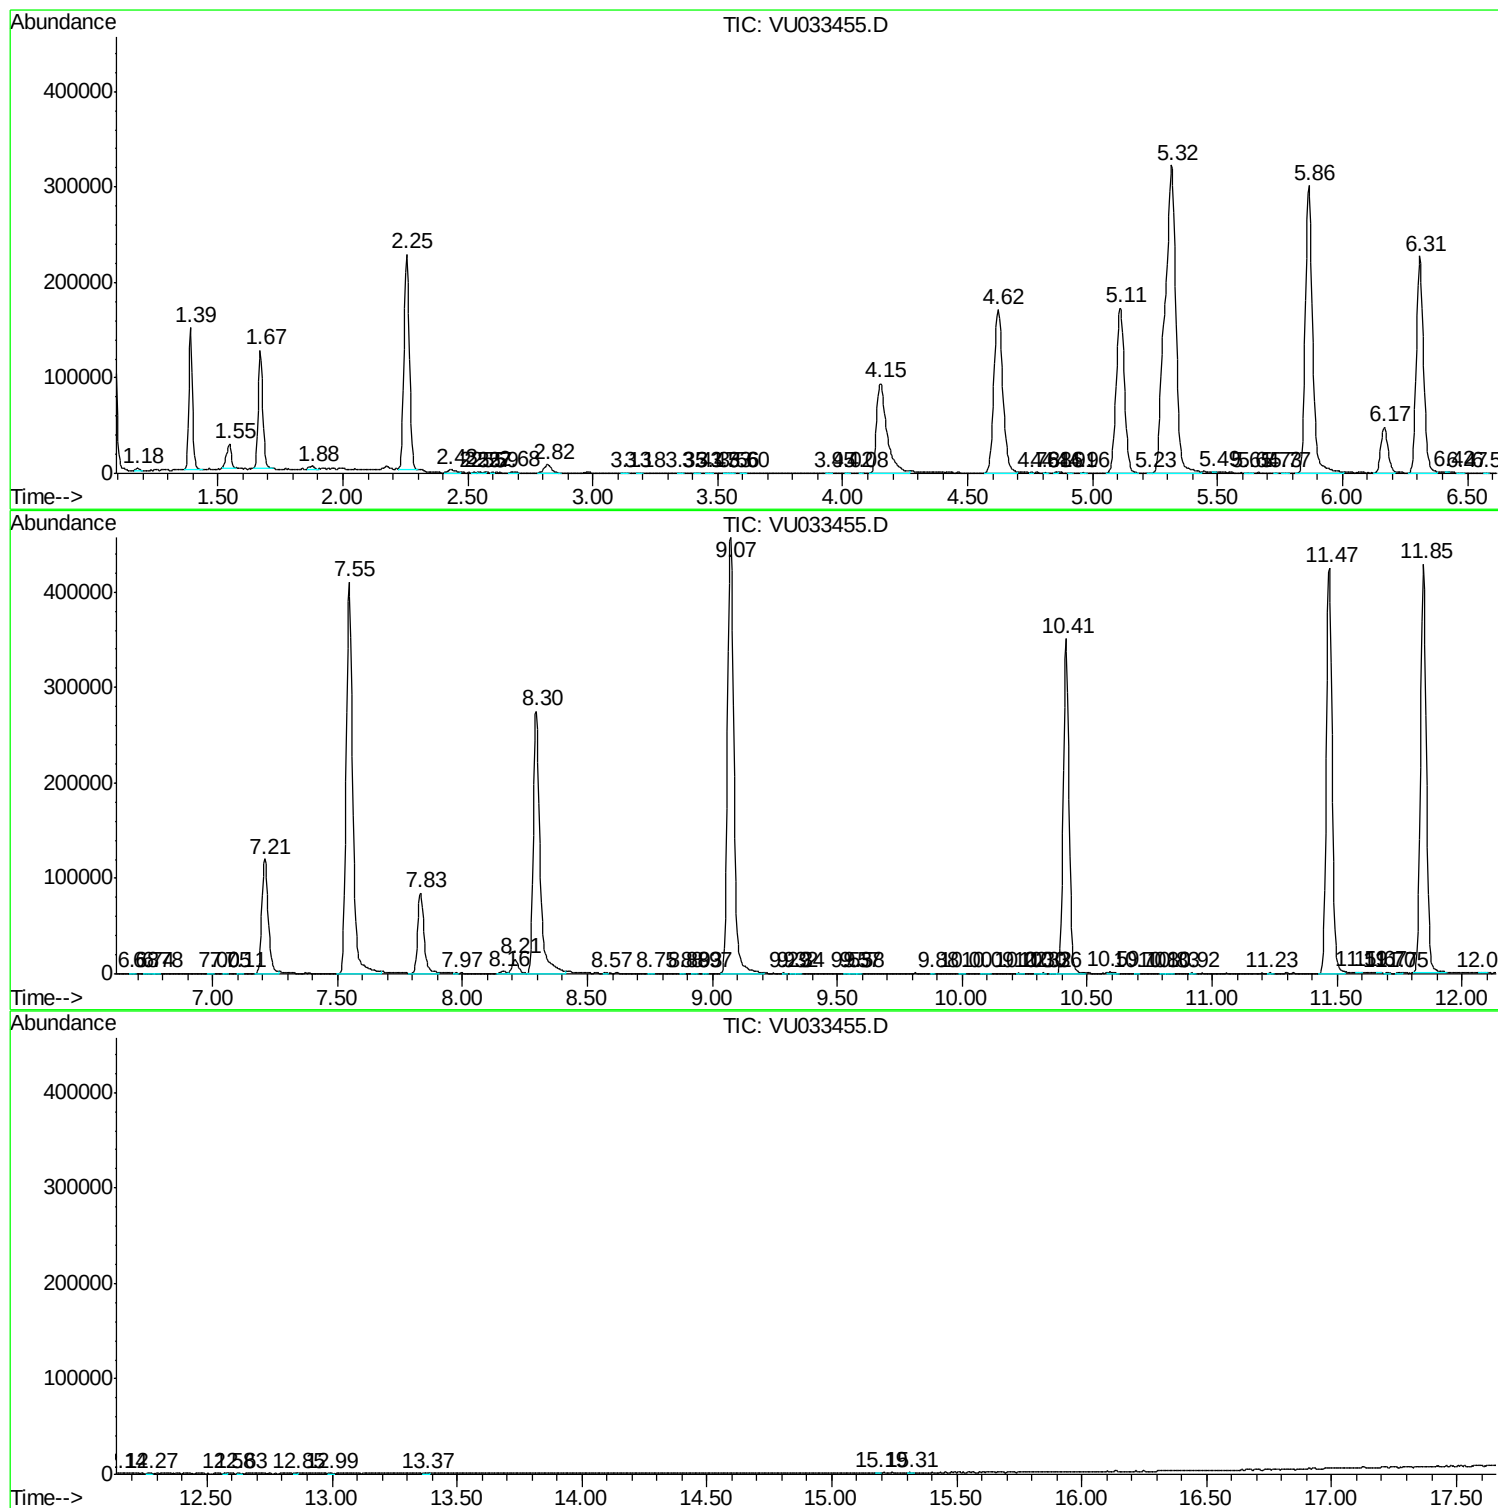

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU072619\
Data File : VU033455.D
Acq On : 26 Jul 2019 15:56
Operator : JC/SP
Sample : K3976-17DL 4X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1










Instrument :
MSVOA_U
ClientSampleId :
C0CC5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.	
1.55	2.61 ug/L	31922	1,4-Difluorobenzene	5.86	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Propanamine	59	C3H9N	000075-31-0	9
2	Ethanol, 2-(methylamino)-	75	C3H9NO	000109-83-1	9
3	Cyanoacetylurea	127	C4H5N3O2	001448-98-2	9
4	l-Alanine, N-(1-oxopentyl)-, met...	187	C9H17NO3	042167-45-3	9
5	1-Propanol, 2-amino-, (S)-	75	C3H9NO	002749-11-3	9

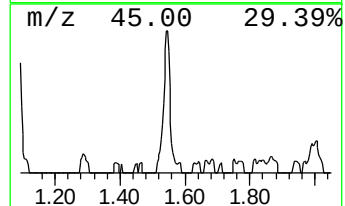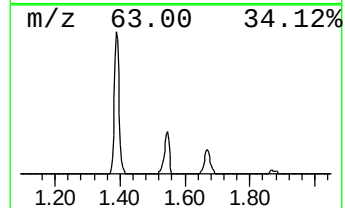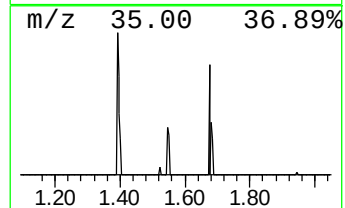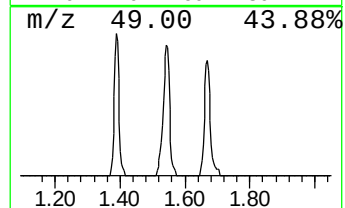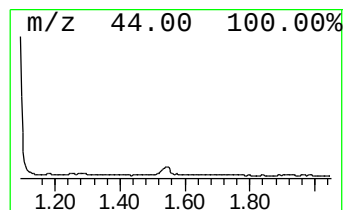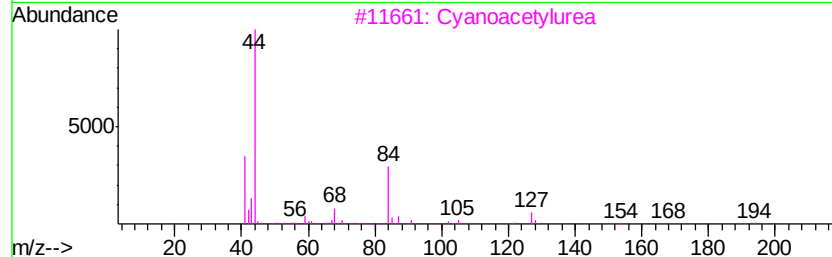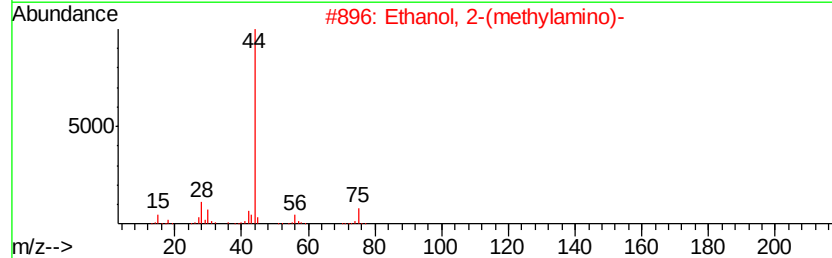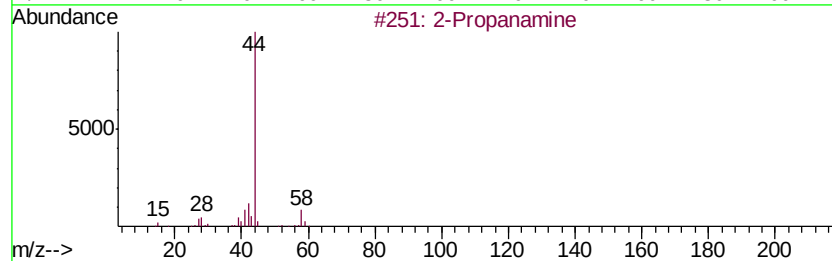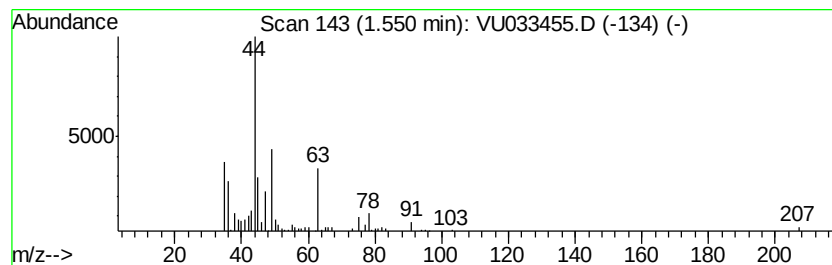

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU072619\
Data File : VU033455.D
Acq On : 26 Jul 2019 15:56
Operator : JC/SP
Sample : K3976-17DL 4X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CC5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown-01	1.55	2.6	ug/L	31922	1	5.86	611853	50.0