


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU072619\
 Data File : VU033439.D
 Acq On : 26 Jul 2019 08:18
 Operator : JC/SP
 Sample : BFB39
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB39

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071219WMA.M
 Title : VOC Analysis
 Last Update : Mon Jul 29 01:55:57 2019

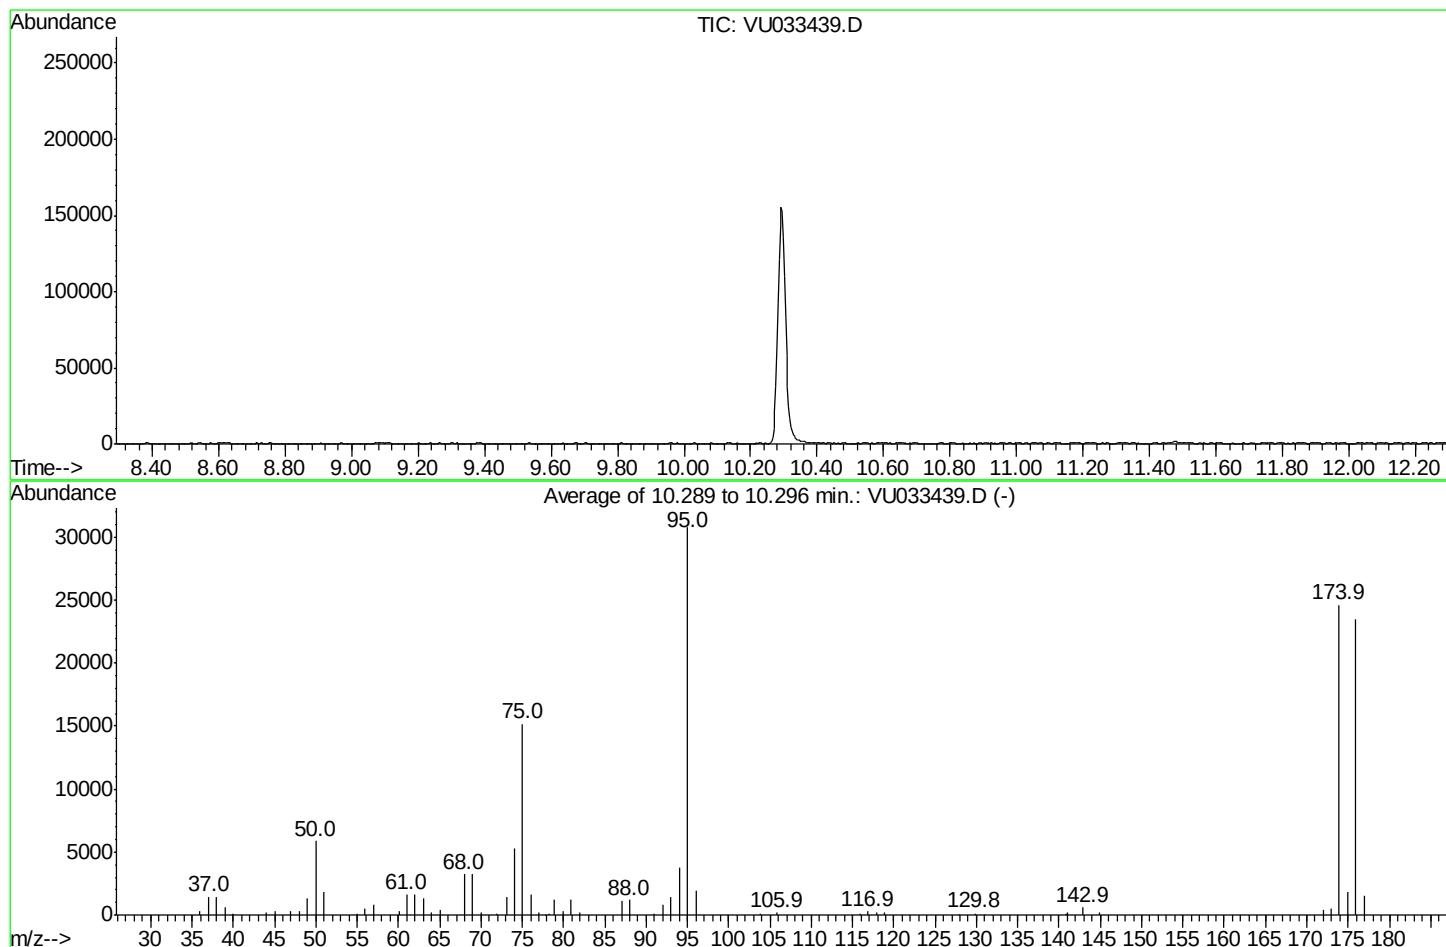

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2850

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	5863	PASS
75	95	30	80	49.3	15185	PASS
95	95	100	100	100.0	30786	PASS
96	95	5	9	6.4	1981	PASS
173	174	0.00	2	1.9	465	PASS
174	95	50	120	80.0	24640	PASS
175	174	5	9	7.6	1880	PASS
176	174	95	101	95.3	23493	PASS
177	176	5	9	6.3	1489	PASS

Scan 2850 (10.254 min): VU033439.D
BFB39

m/z	Abundance
40.00	134.0
44.00	235.0

Instrument :
MSVOA_U
ClientSampleId :
BFB39

m/z	Abundance
35.90	263.0
37.00	1405.0
38.00	1429.0
39.00	592.0
39.90	193.0
44.00	408.0
45.00	275.0
46.90	248.0
48.00	297.0
49.00	1254.0
50.00	5722.0
51.00	1866.0
55.90	490.0
57.00	822.0
60.00	272.0
61.00	1464.0
62.00	1608.0
63.00	1241.0
63.90	248.0
65.10	322.0
68.00	3033.0
69.00	3112.0
70.10	184.0
72.00	148.0
73.00	1425.0
74.00	5382.0
75.00	14556.0
76.00	1562.0
77.00	244.0
78.90	1166.0
79.90	321.0
80.90	1149.0
81.90	231.0
87.00	1057.0
87.90	1195.0
91.00	114.0
92.00	916.0
93.00	1369.0
94.00	3456.0
95.00	29216.0
96.00	1928.0
103.80	108.0
105.90	187.0
115.90	156.0
116.90	263.0
117.90	192.0
118.90	155.0
129.90	140.0
130.90	100.0
141.10	242.0
142.90	525.0
144.90	167.0
172.00	381.0
173.00	447.0
174.00	23024.0
175.00	1795.0
175.90	22440.0
176.90	1471.0

Instrument :
MSVOA_U
ClientSampleId :
BFB39

m/z	Abundance
35.90	297.0
37.00	1501.0
38.00	1493.0
39.00	599.0
39.90	206.0
44.00	417.0
45.00	296.0
47.00	259.0
47.90	289.0
49.00	1413.0
50.00	6092.0
51.00	1902.0
55.90	505.0
57.00	854.0
60.00	346.0
61.00	1634.0
62.00	1680.0
63.00	1326.0
63.90	259.0
65.10	377.0
68.00	3304.0
69.00	3365.0
70.10	212.0
72.00	160.0
73.00	1493.0
74.00	5531.0
75.00	15642.0
76.00	1672.0
77.00	255.0
78.20	144.0
78.90	1229.0
79.90	331.0
80.90	1291.0
82.00	226.0
87.00	1164.0
88.00	1245.0
91.00	122.0
92.00	881.0
93.00	1496.0
94.00	3834.0
95.00	31864.0
96.00	2034.0
103.80	120.0
105.90	215.0
115.90	170.0
116.90	259.0
117.90	162.0
118.90	194.0
129.90	162.0
140.80	234.0
141.10	239.0
142.90	597.0
144.90	157.0
172.00	429.0
173.00	488.0
174.00	25456.0
175.00	1897.0
175.90	24232.0
176.90	1553.0

Instrument :
MSVOA_U
ClientSampleId :
BFB39

m/z	Abundance
35.90	314.0
37.10	1450.0
38.00	1366.0
39.00	579.0
39.90	195.0
44.00	440.0
45.00	281.0
47.10	271.0
47.90	198.0
49.00	1389.0
50.00	5777.0
51.00	1789.0
55.00	170.0
55.90	475.0
57.00	801.0
60.10	347.0
61.00	1661.0
62.00	1631.0
63.00	1310.0
63.90	253.0
65.10	405.0
68.00	3330.0
69.00	3187.0
70.00	211.0
71.90	150.0
73.10	1374.0
74.00	5105.0
75.00	15359.0
76.00	1623.0
77.00	240.0
77.80	114.0
78.20	129.0
78.90	1236.0
79.90	314.0
80.90	1296.0
82.10	209.0
87.00	1148.0
88.00	1140.0
91.00	111.0
92.00	761.0
93.00	1490.0
94.00	3880.0
95.00	31280.0
96.00	1982.0
103.80	127.0
105.90	195.0
115.90	126.0
116.90	253.0
117.90	149.0
118.90	204.0
127.90	108.0
129.80	134.0
141.00	250.0
142.90	616.0
144.90	164.0
171.90	473.0
173.00	461.0
173.90	25440.0
175.00	1950.0
175.90	23808.0
176.90	1445.0

Instrument :
MSVOA_U
ClientSampleId :
BFB39