

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072622\
 Data File : VU049907.D
 Acq On : 26 Jul 2022 11:53
 Operator : SY/MD
 Sample : VU0726WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK098

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049907.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	90	rBV	44769	50392	10.16%	1.584%
2	1.912	169	178	193	rBV	44834	55342	11.15%	1.739%
3	2.565	369	381	400	rVB	70519	115926	23.36%	3.644%
4	3.044	520	530	545	rVB2	12338	21518	4.34%	0.676%
5	4.642	1013	1027	1073	rBV2	60825	232355	46.83%	7.303%
6	5.063	1142	1158	1176	rBV3	74694	167964	33.85%	5.279%
7	5.726	1340	1364	1389	rBV3	140131	370864	74.75%	11.657%
8	6.250	1513	1527	1544	rBV	118011	225282	45.41%	7.081%
9	6.536	1604	1616	1627	rBV8	2632	5117	1.03%	0.161%
10	6.690	1651	1664	1687	rBV	93010	182969	36.88%	5.751%
11	7.565	1925	1936	1953	rBV	39296	71729	14.46%	2.255%
12	7.899	2027	2040	2056	rBV	143783	251717	50.73%	7.912%
13	8.182	2117	2128	2141	rBV	25217	43623	8.79%	1.371%
14	8.639	2256	2270	2301	rBV2	196287	496156	100.00%	15.595%
15	9.417	2499	2512	2532	rBV	163457	283177	57.07%	8.901%
16	10.754	2917	2928	2947	rVB2	78197	127856	25.77%	4.019%
17	11.812	3245	3257	3276	rBV	151759	245699	49.52%	7.723%
18	12.195	3363	3376	3395	rBV	134216	222260	44.80%	6.986%
19	14.095	3953	3967	3982	rBV	3441	6529	1.32%	0.205%
20	14.333	4032	4041	4052	rVB5	3541	5079	1.02%	0.160%




Sum of corrected areas: 3181554

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072622\
Data File : VU049907.D
Acq On : 26 Jul 2022 11:53
Operator : SY/MD
Sample : VU0726WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK098

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

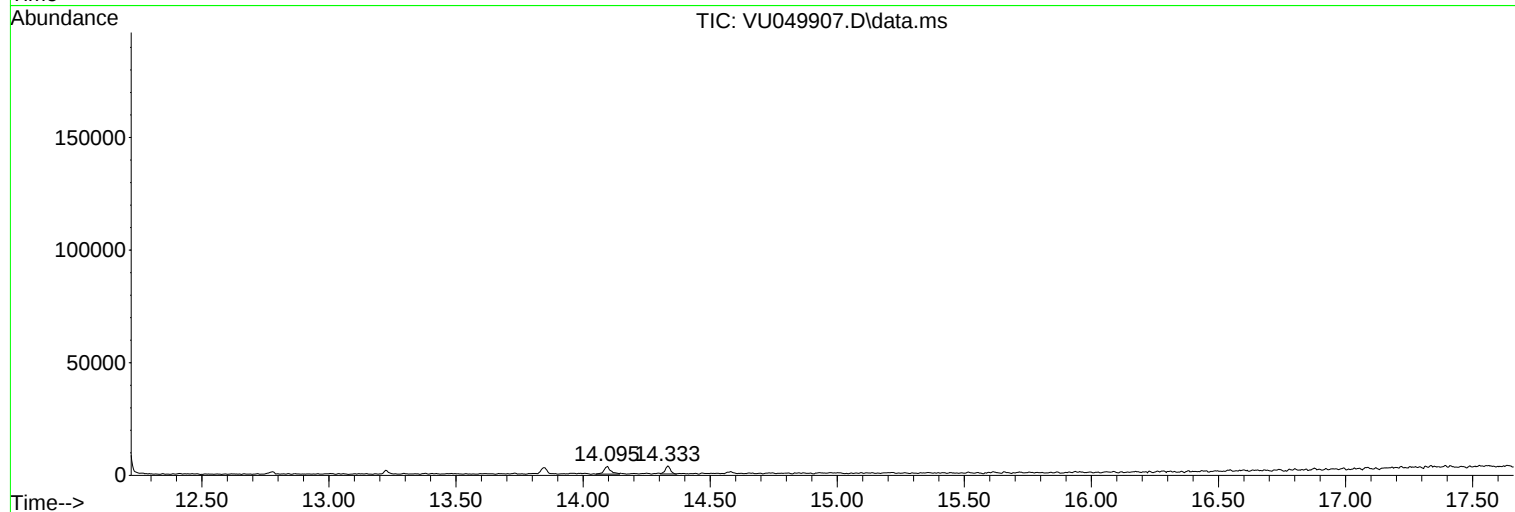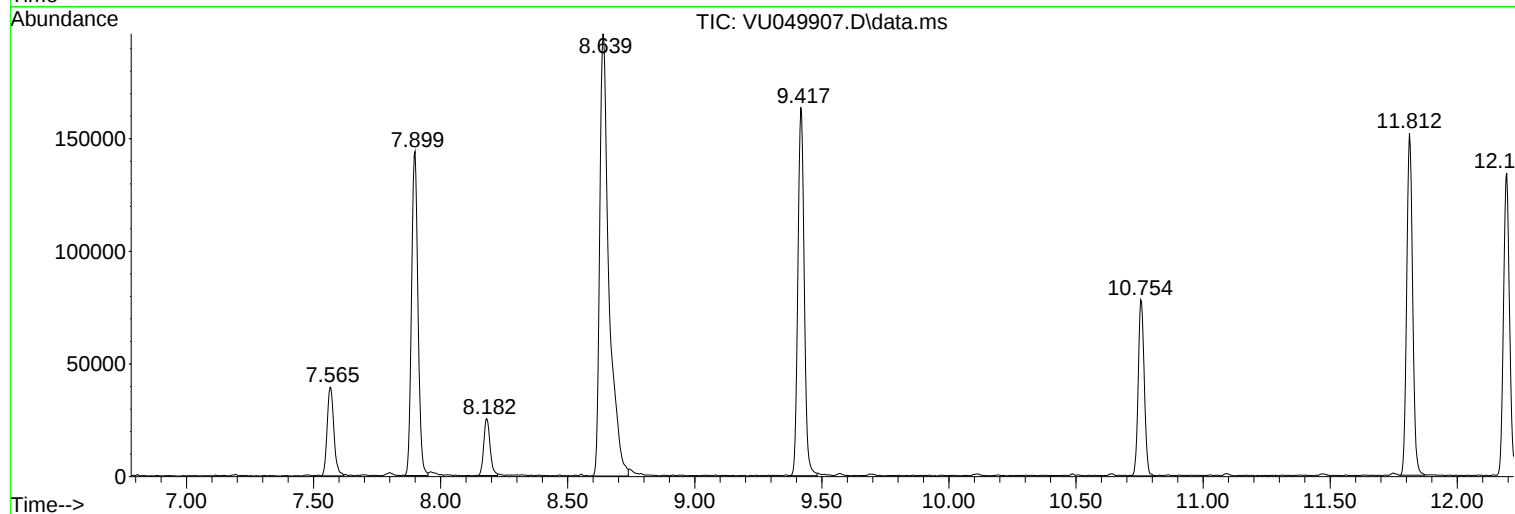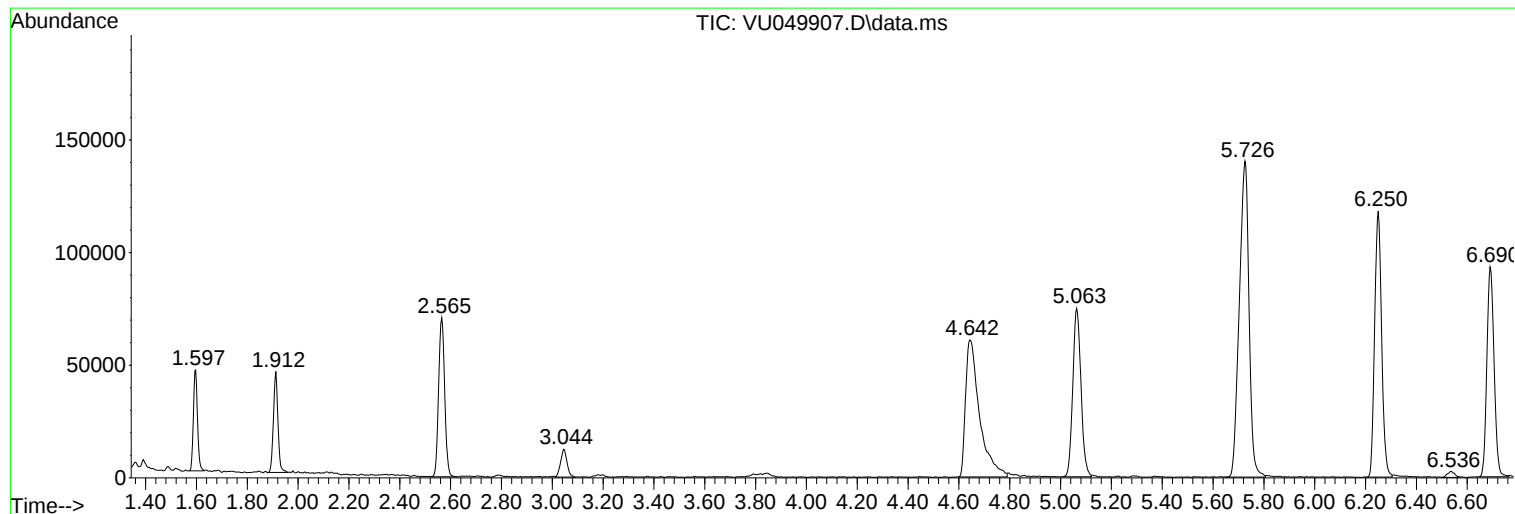

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072622\
Data File : VU049907.D
Acq On : 26 Jul 2022 11:53
Operator : SY/MD
Sample : VU0726WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK098

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072622\
Data File : VU049907.D
Acq On : 26 Jul 2022 11:53
Operator : SY/MD
Sample : VU0726WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK098

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc