

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072622\
 Data File : VU049923.D
 Acq On : 26 Jul 2022 19:37
 Operator : SY/MD
 Sample : N3870-11DL 25X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBJ10DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049923.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.594	73	79	90	rVB	39095	43062	8.18%	1.143%
2	1.729	114	121	131	rVB	7771	9785	1.86%	0.260%
3	1.912	169	178	188	rBV	36661	46788	8.88%	1.242%
4	2.565	367	381	400	rVB	65939	111611	21.19%	2.964%
5	3.044	513	530	549	rVB2	14235	28675	5.45%	0.761%
6	3.182	560	573	590	rBV	12367	26965	5.12%	0.716%
7	4.652	1011	1030	1095	rBV4	83218	352801	67.00%	9.368%
8	5.063	1143	1158	1188	rVB	75645	174411	33.12%	4.631%
9	5.726	1343	1364	1383	rBV2	132689	352247	66.89%	9.353%
10	6.250	1508	1527	1545	rBV	108068	204704	38.87%	5.435%
11	6.542	1603	1618	1638	rBV	269340	511640	97.16%	13.586%
12	6.690	1651	1664	1682	rVB	92894	179813	34.15%	4.775%
13	7.568	1924	1937	1955	rBV2	38006	68986	13.10%	1.832%
14	7.899	2026	2040	2057	rBV	135973	239300	45.44%	6.354%
15	8.179	2117	2127	2144	rBV2	23086	40703	7.73%	1.081%
16	8.639	2257	2270	2312	rBV3	201115	526601	100.00%	13.983%
17	9.417	2497	2512	2533	rBV	151492	259739	49.32%	6.897%
18	10.758	2915	2929	2947	rBV	80703	131076	24.89%	3.480%
19	11.812	3245	3257	3275	rBV	142167	228669	43.42%	6.072%
20	12.195	3361	3376	3398	rBV	140183	228485	43.39%	6.067%




Sum of corrected areas: 3766061

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072622\
Data File : VU049923.D
Acq On : 26 Jul 2022 19:37
Operator : SY/MD
Sample : N3870-11DL 25X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBJ10DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

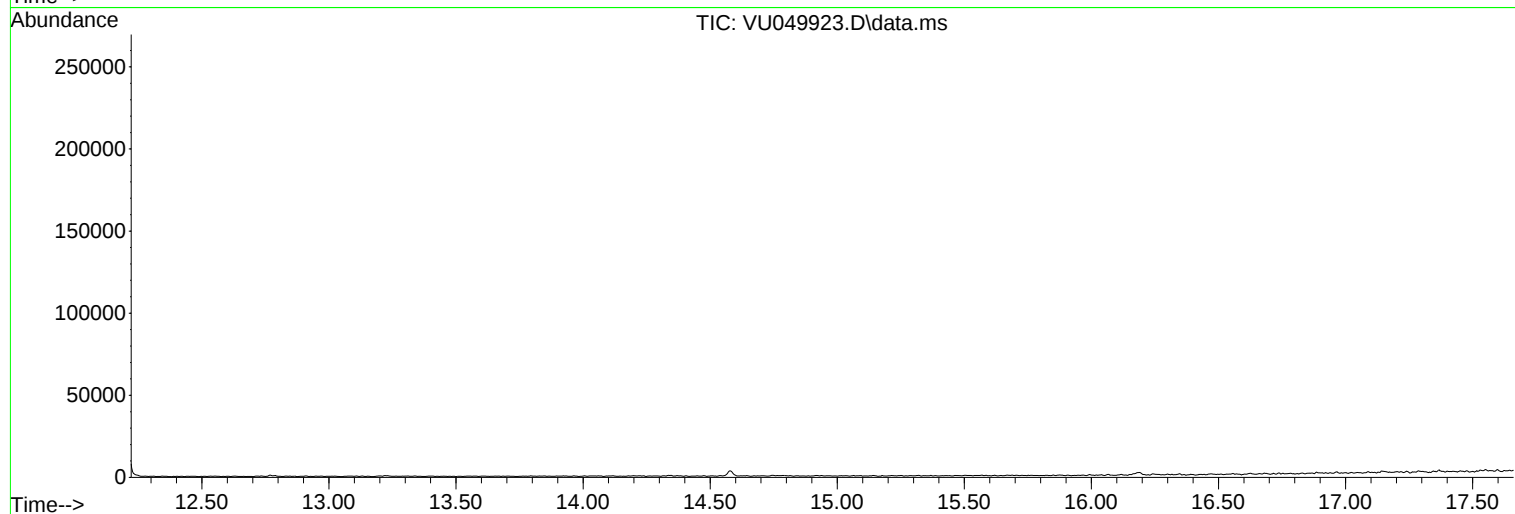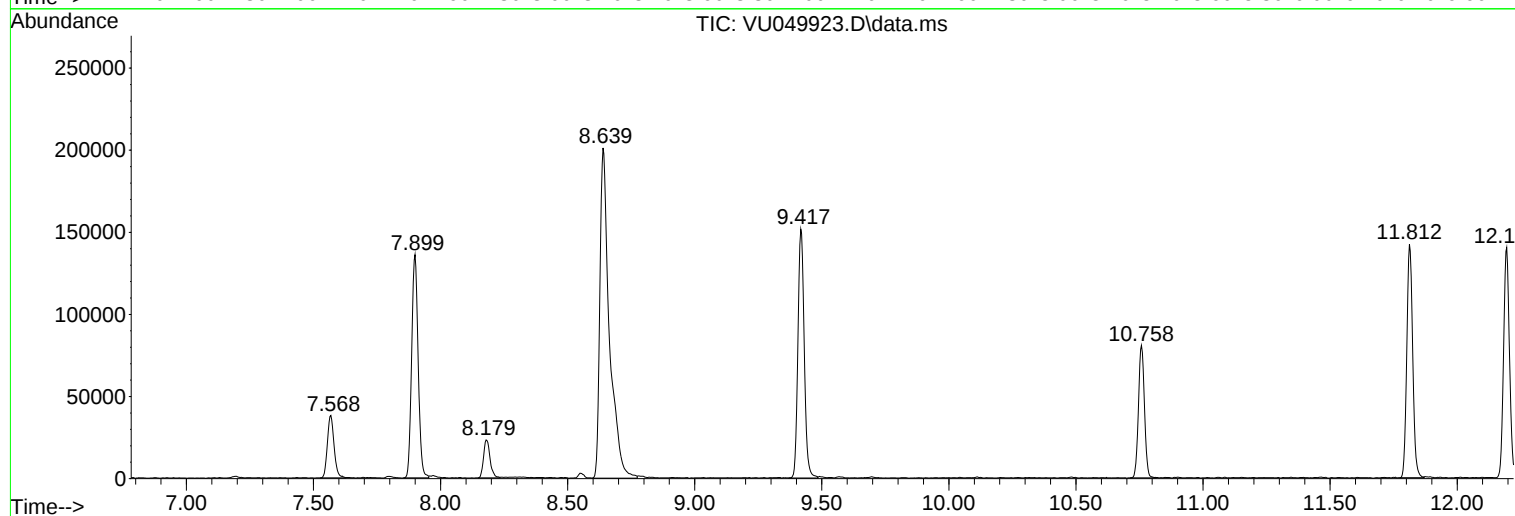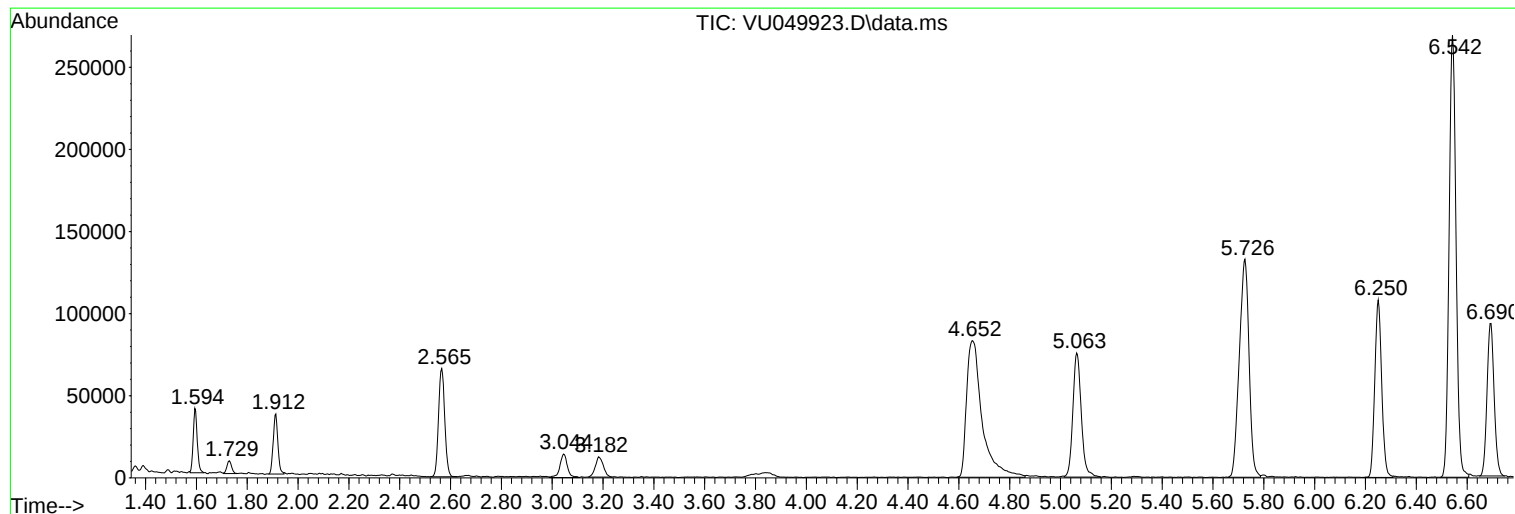

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072622\
Data File : VU049923.D
Acq On : 26 Jul 2022 19:37
Operator : SY/MD
Sample : N3870-11DL 25X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBJ10DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072622\
Data File : VU049923.D
Acq On : 26 Jul 2022 19:37
Operator : SY/MD
Sample : N3870-11DL 25X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBJ10DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc