

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072622\
 Data File : VU049941.D
 Acq On : 27 Jul 2022 03:48
 Operator : SY/MD
 Sample : N3879-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUH6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049941.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.359	3	6	10	rVV	8915	6923	1.29%	0.201%
2	1.385	11	14	29	rVB3	5145	7423	1.38%	0.215%
3	1.597	72	80	93	rVB	35855	40984	7.61%	1.190%
4	1.912	170	178	194	rVB	32564	41768	7.76%	1.212%
5	2.137	241	248	259	rVB	14808	22243	4.13%	0.646%
6	2.568	371	382	395	rBV	49435	78944	14.66%	2.291%
7	4.636	1008	1025	1063	rBV	78446	240927	44.76%	6.993%
8	5.063	1144	1158	1179	rBV2	66504	155755	28.93%	4.521%
9	5.726	1344	1364	1391	rBV3	114915	316855	58.86%	9.196%
10	6.250	1513	1527	1544	rBV	90450	169578	31.50%	4.922%
11	6.542	1606	1618	1633	rVB3	26639	48307	8.97%	1.402%
12	6.690	1651	1664	1691	rBV	84681	166061	30.85%	4.820%
13	7.568	1925	1937	1953	rBV	32239	57471	10.68%	1.668%
14	7.899	2027	2040	2056	rBV	117809	203880	37.87%	5.917%
15	8.179	2118	2127	2145	rBV3	20621	36153	6.72%	1.049%
16	8.552	2230	2243	2258	rBV	300455	504384	93.70%	14.639%
17	8.639	2258	2270	2312	rVV5	212370	538317	100.00%	15.624%
18	9.417	2500	2512	2536	rBV	131670	231089	42.93%	6.707%
19	10.754	2917	2928	2954	rBV	90997	160438	29.80%	4.657%
20	11.812	3244	3257	3271	rBV	124439	204244	37.94%	5.928%
21	12.192	3361	3375	3395	rBV	128672	213699	39.70%	6.202%




Sum of corrected areas: 3445443

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072622\
Data File : VU049941.D
Acq On : 27 Jul 2022 03:48
Operator : SY/MD
Sample : N3879-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

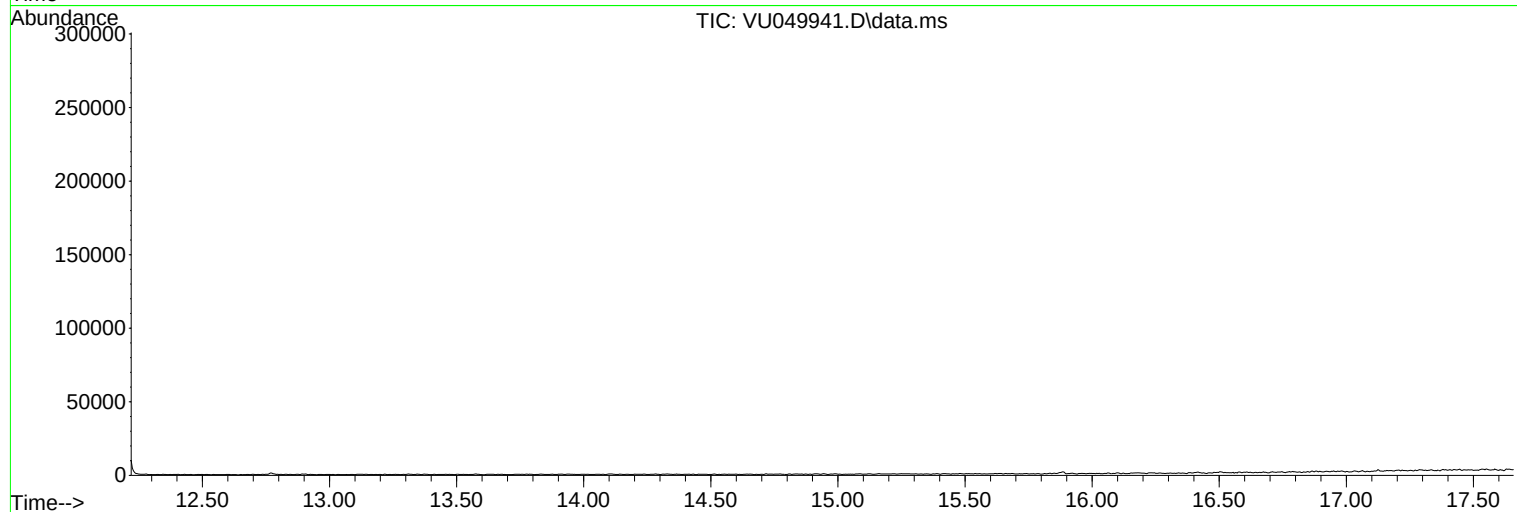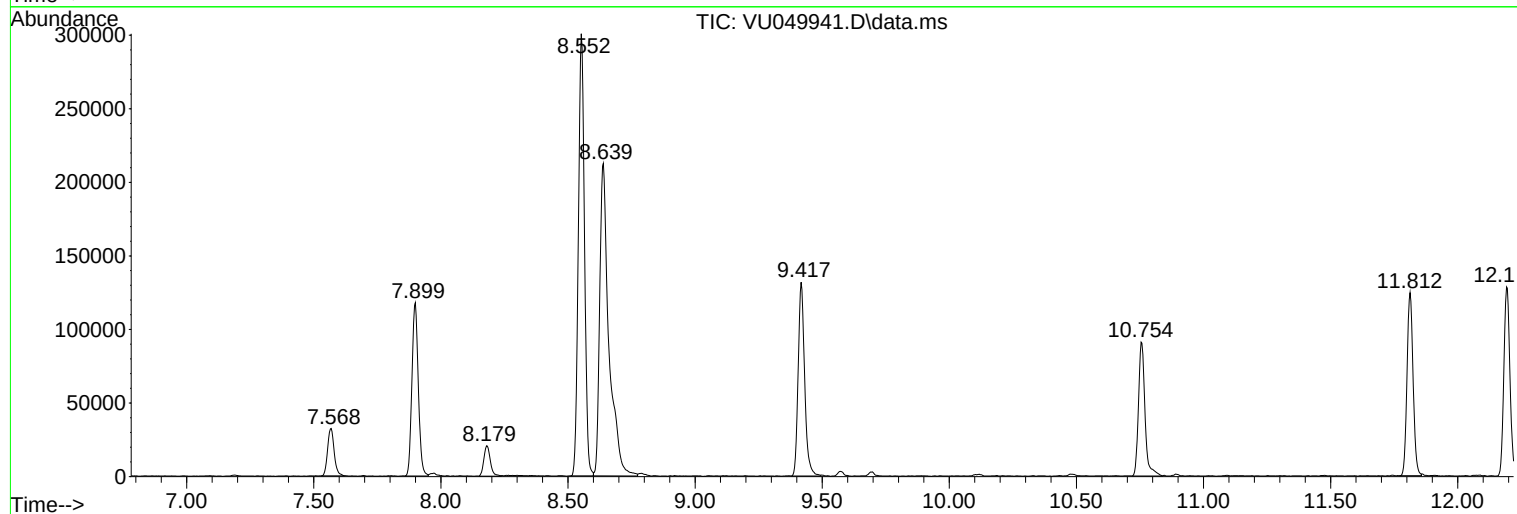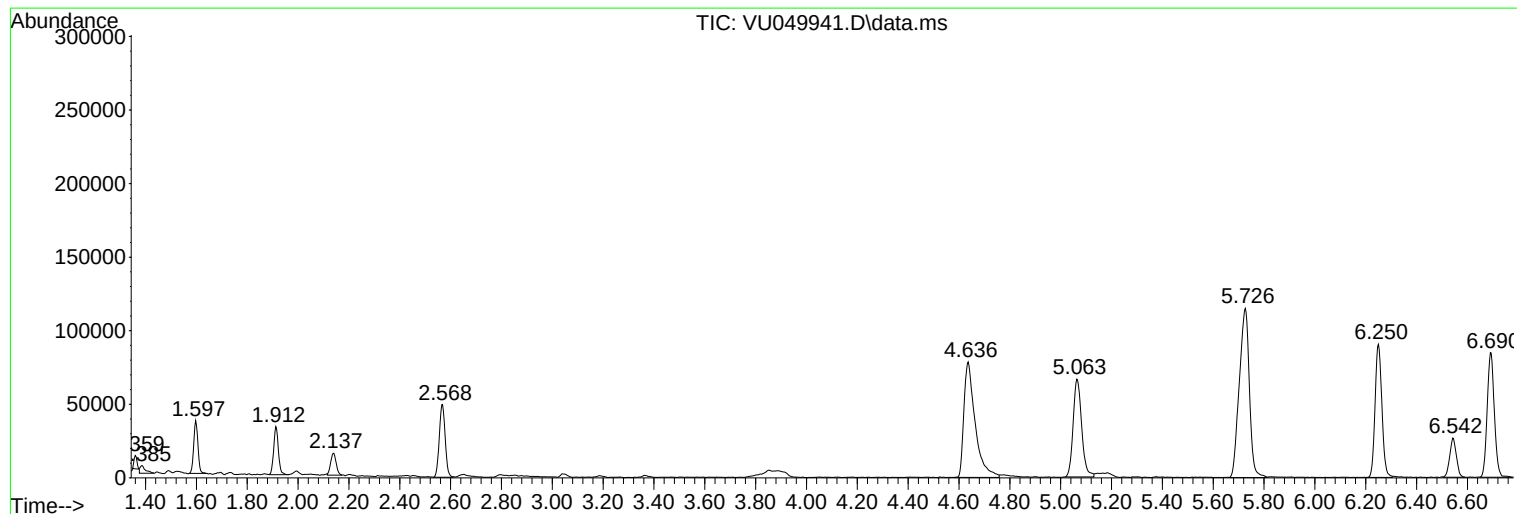

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072622\
Data File : VU049941.D
Acq On : 27 Jul 2022 03:48
Operator : SY/MD
Sample : N3879-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072622\
Data File : VU049941.D
Acq On : 27 Jul 2022 03:48
Operator : SY/MD
Sample : N3879-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc