


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072622\
 Data File : VU049905.D
 Acq On : 26 Jul 2022 10:08
 Operator : SY/MD
 Sample : BFB094
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB094

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072222WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Jul 27 05:17:43 2022

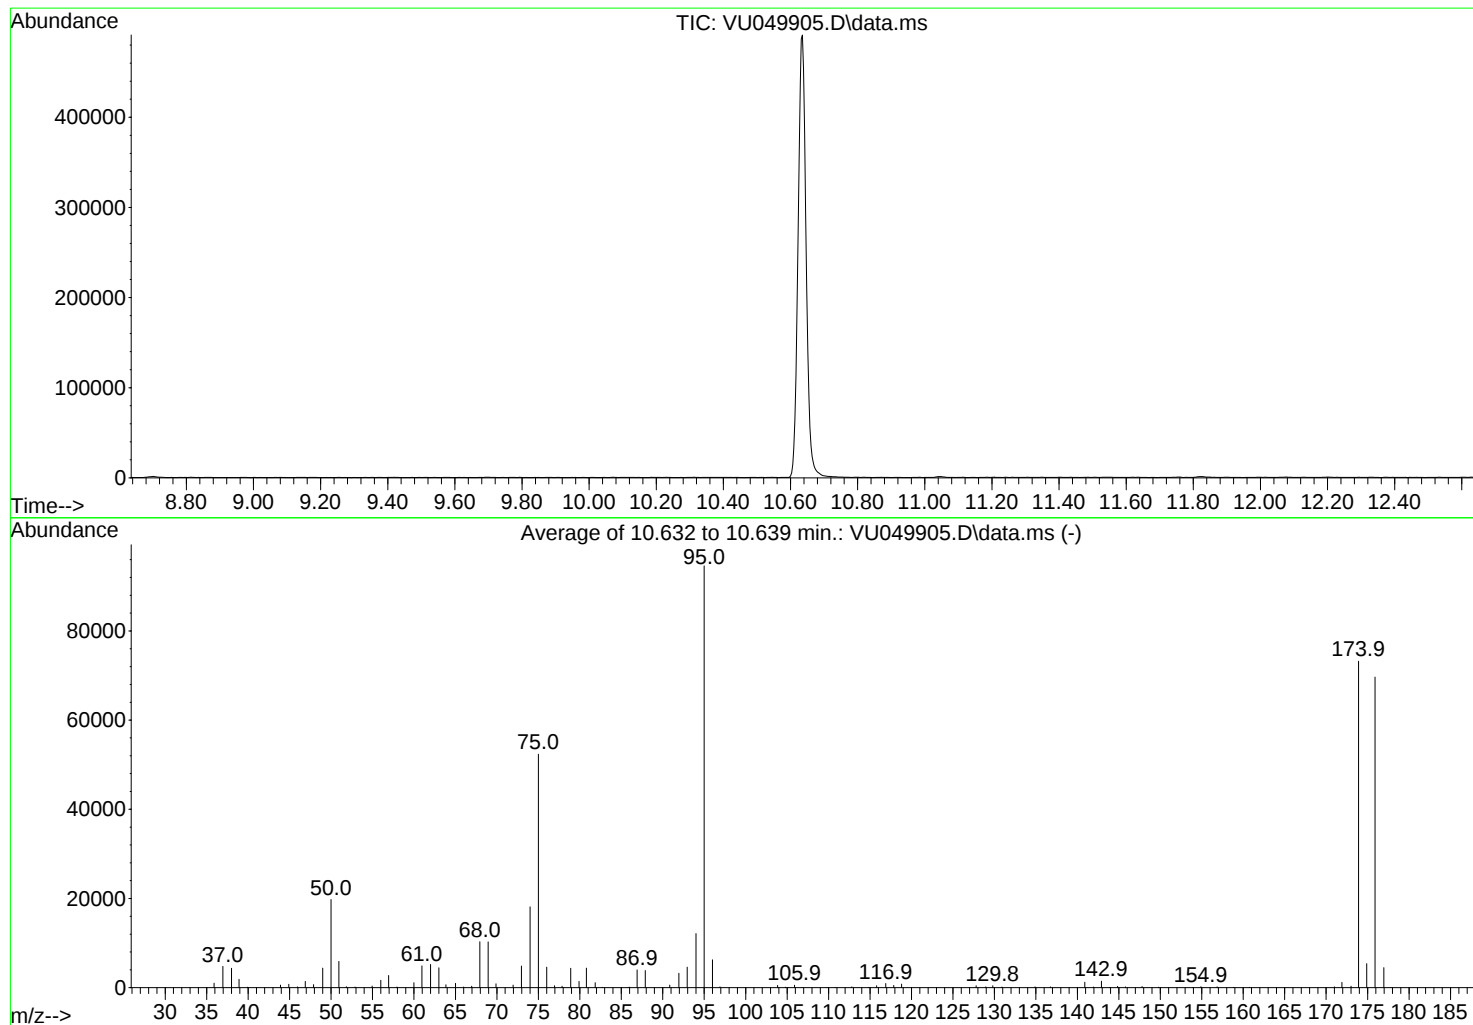

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	19760	PASS
75	95	30	80	55.3	52355	PASS
95	95	100	100	100.0	94600	PASS
96	95	5	9	6.6	6243	PASS
173	174	0.00	2	0.5	330	PASS
174	95	50	120	77.4	73197	PASS
175	174	5	9	7.4	5394	PASS
176	174	95	101	95.1	69643	PASS
177	176	5	9	6.4	4476	PASS

m/z	Abundance
39.90	156.0
43.90	361.0

Instrument :
MSVOA_U
ClientSampleId :
BFB094

m/z	Abundance
35.90	1071.0
37.00	5143.0
38.00	4596.0
38.90	1964.0
39.90	291.0
43.90	975.0
44.90	796.0
45.90	216.0
46.90	1307.0
48.00	740.0
49.00	4297.0
50.00	20632.0
50.90	5955.0
51.90	222.0
52.90	118.0
55.00	417.0
56.00	1671.0
57.00	3110.0
58.00	136.0
60.00	1164.0
61.00	5107.0
62.00	5144.0
63.00	4558.0
63.80	657.0
65.00	1030.0
66.00	139.0
66.90	325.0
67.90	10150.0
69.00	10399.0
69.90	863.0
71.90	624.0
73.00	5028.0
74.00	18776.0
75.00	53648.0
76.00	4803.0
77.00	411.0
77.90	350.0
78.90	4543.0
79.90	1425.0
80.80	4486.0
81.80	1178.0
82.70	117.0
85.80	209.0
86.90	4102.0
87.90	4212.0
90.80	580.0
91.90	3328.0
93.00	4976.0
94.00	12305.0
95.00	97048.0
96.00	6442.0
96.90	234.0
103.90	476.0
104.80	158.0
105.90	585.0
106.80	109.0
112.80	159.0
114.80	112.0
115.80	409.0
116.90	911.0
117.80	523.0
118.80	817.0
127.80	451.0
129.00	219.0
129.80	423.0
130.90	145.0
134.90	229.0
136.80	222.0
140.90	1257.0
141.90	149.0
142.90	1484.0
144.90	285.0
145.80	168.0
147.80	233.0
149.80	167.0
153.90	127.0
154.90	221.0
156.80	187.0
160.70	104.0
171.00	165.0
171.90	1218.0
173.90	73520.0
174.90	5612.0
175.90	69440.0
177.00	4344.0
177.80	114.0

Instrument :
MSVOA_U
ClientSampleId :
BFB094

m/z	Abundance
35.90	1013.0
37.00	4845.0
38.00	4504.0
38.90	1890.0
39.90	274.0
43.90	976.0
44.90	755.0
46.00	194.0
46.90	1528.0
47.90	665.0
49.00	4521.0
50.00	20480.0
51.00	6018.0
51.80	231.0
52.90	137.0
55.00	374.0
56.00	1710.0
57.00	2758.0
57.90	145.0
60.00	1107.0
60.90	5054.0
62.00	5359.0
63.00	4547.0
63.90	669.0
65.00	997.0
66.00	144.0
66.90	318.0
68.00	10593.0
68.90	10492.0
69.90	897.0
72.00	570.0
73.00	4952.0
74.00	18616.0
75.00	54168.0
76.00	4766.0
76.90	440.0
77.80	362.0
78.90	4489.0
79.90	1405.0
80.80	4534.0
81.80	1131.0
82.70	102.0
86.00	189.0
86.90	4117.0
87.90	3961.0
90.90	596.0
92.00	3332.0
92.90	4675.0
94.00	12484.0
95.00	97368.0
96.00	6386.0
96.90	187.0
103.80	526.0
104.80	125.0
105.90	562.0
112.80	186.0
115.80	454.0
116.90	994.0
117.90	499.0
118.80	819.0
127.80	441.0
129.00	189.0
129.80	477.0
130.90	160.0
134.90	213.0
136.80	186.0
140.90	1237.0
141.90	166.0
142.90	1444.0
144.80	284.0
145.80	184.0
147.80	255.0
149.80	129.0
154.90	226.0
156.80	175.0
158.90	102.0
160.80	104.0
171.00	203.0
171.90	1226.0
173.90	75776.0
174.90	5536.0
175.90	71664.0
176.90	4626.0

Instrument :
MSVOA_U
ClientSampleId :
BFB094

m/z	Abundance
35.90	887.0
36.90	4305.0
38.00	3904.0
38.90	1803.0
39.90	242.0
43.90	840.0
44.90	669.0
46.00	117.0
46.90	1373.0
47.80	613.0
49.00	4329.0
50.00	18168.0
51.00	5646.0
51.80	239.0
52.90	133.0
54.90	310.0
56.00	1623.0
56.90	2345.0
57.90	103.0
60.00	1113.0
60.90	4451.0
62.00	5127.0
63.00	4266.0
63.90	629.0
65.00	888.0
66.00	105.0
67.00	291.0
68.00	10140.0
68.90	9896.0
69.90	830.0
72.00	536.0
72.90	4525.0
74.00	16936.0
75.00	49248.0
76.00	4196.0
76.90	443.0
77.80	291.0
78.90	3970.0
79.90	1354.0
80.80	4132.0
81.90	993.0
86.00	153.0
86.90	3755.0
87.90	3372.0
90.90	573.0
92.00	3029.0
93.00	4115.0
94.00	11609.0
95.00	89384.0
96.00	5900.0
96.90	174.0
103.80	502.0
105.10	142.0
105.90	499.0
109.80	114.0
110.80	104.0
112.80	173.0
115.80	419.0
116.90	955.0
117.90	490.0
118.80	696.0
127.80	386.0
128.90	180.0
129.80	450.0
130.90	182.0
134.90	150.0
136.70	149.0
140.90	1201.0
142.00	148.0
142.90	1339.0
143.90	133.0
144.90	305.0
145.80	181.0
147.80	257.0
154.90	190.0
156.90	182.0
158.80	114.0
171.00	159.0
171.90	1111.0
173.00	989.0
173.90	70296.0
174.90	5034.0
175.90	67824.0
176.90	4459.0

Instrument :
MSVOA_U
ClientSampleId :
BFB094