

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072623\
 Data File : VU054877.D
 Acq On : 26 Jul 2023 15:37
 Operator : MD/SY
 Sample : VU0726WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0726WBL01

Quant Time: Jul 28 03:20:53 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Wed Jul 26 09:45:35 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.113	96	27569	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.634	95	8362	1.000	ug/l	0.00
Spiked Amount 1.000			Recovery	=	100.000%	
68) 1,2-Dichlorobenzene-d4	12.193	152	9079	0.961	ug/l	0.00
Spiked Amount 1.000			Recovery	=	96.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072623\
Data File : VU054877.D
Acq On : 26 Jul 2023 15:37
Operator : MD/SY
Sample : VU0726WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0726WBL01

Quant Time: Jul 28 03:20:53 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Wed Jul 26 09:45:35 2023
Response via : Initial Calibration




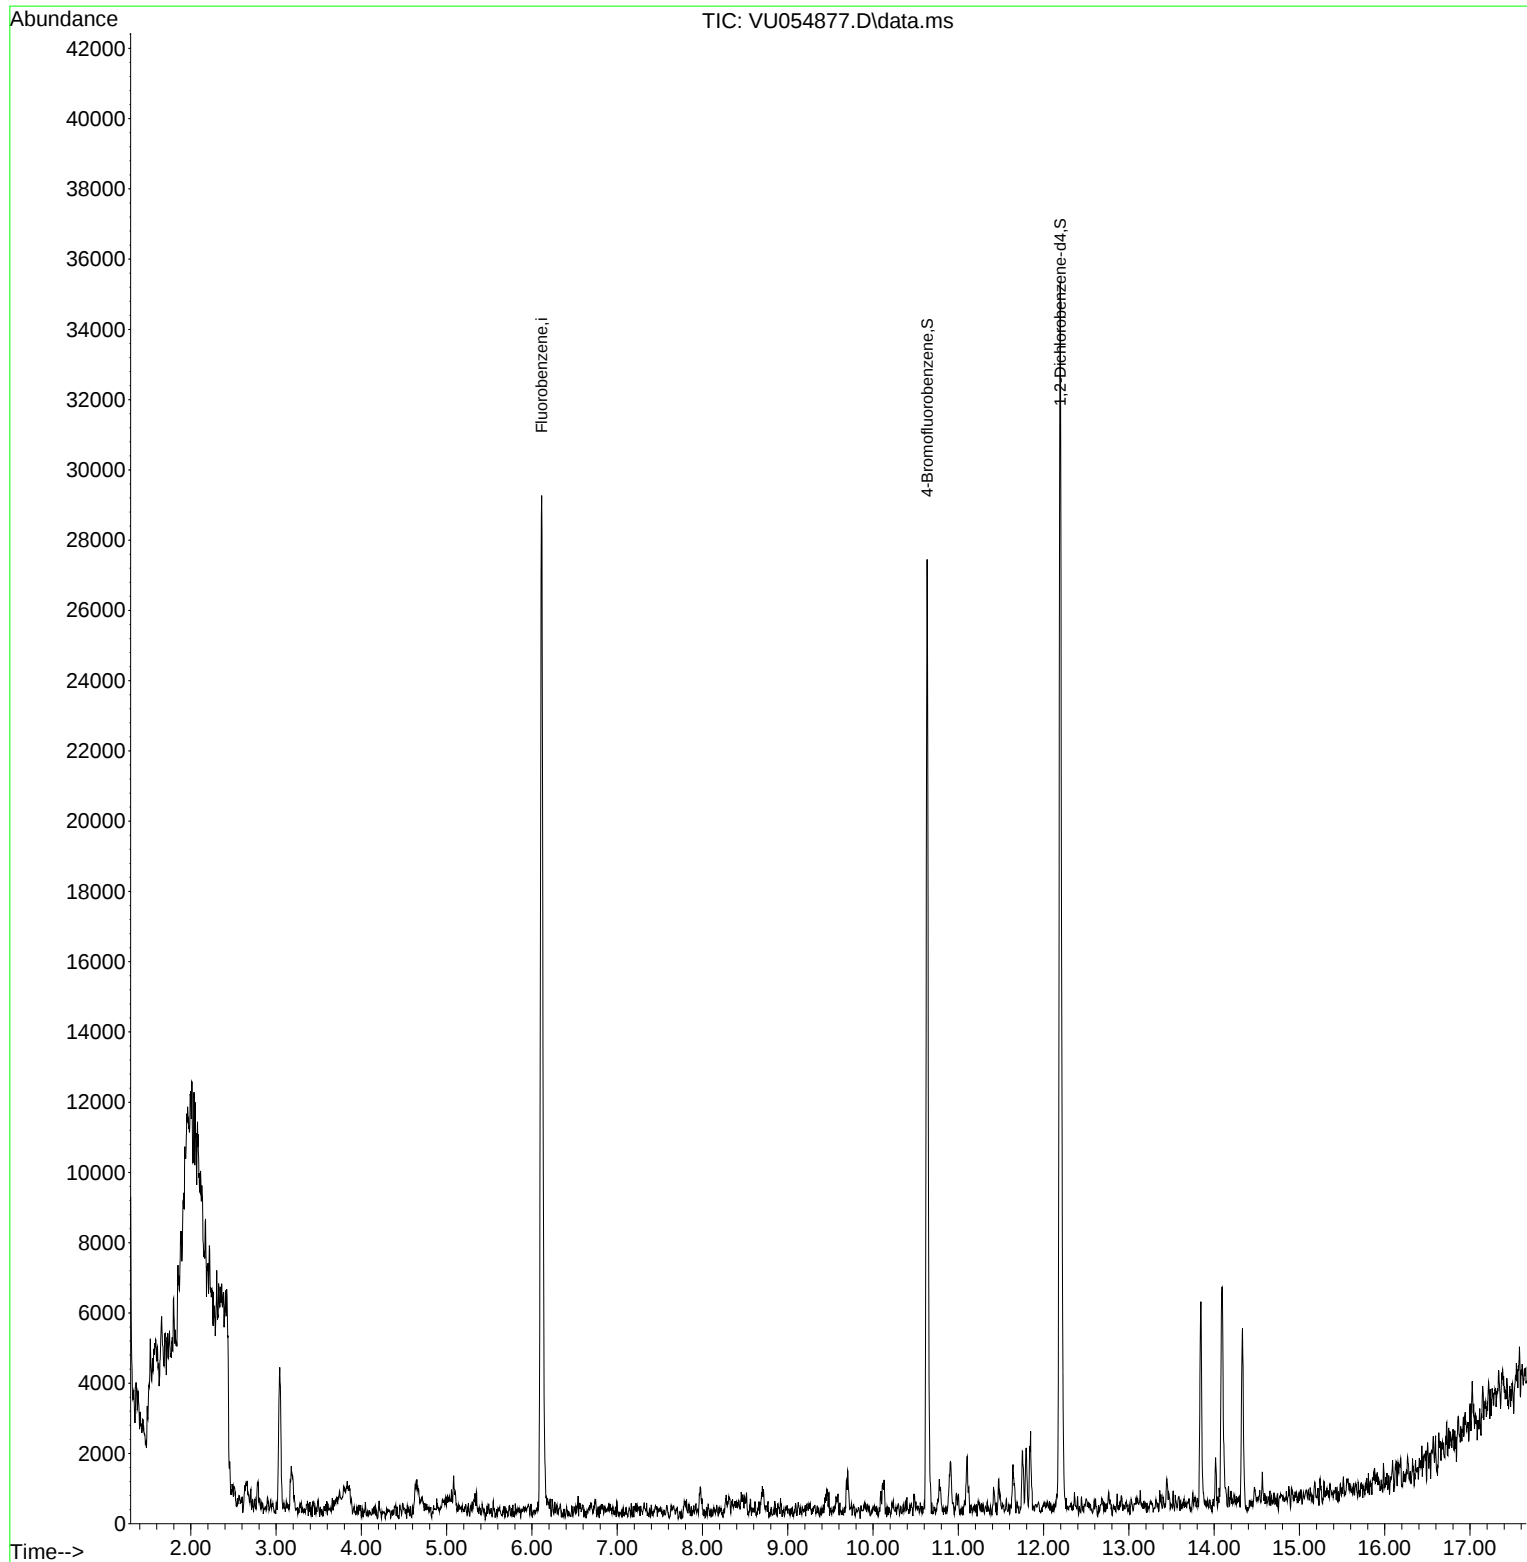


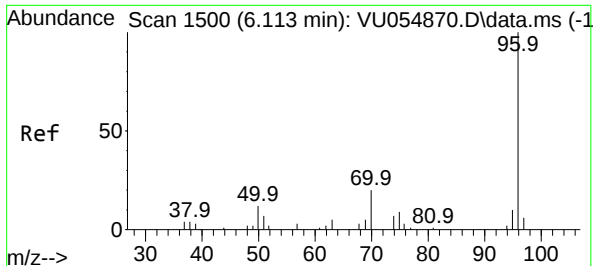

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.113 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU054877.D
Acq: 26 Jul 2023 15:37




Instrument :
MSVOA_U
ClientSampleId :
VU0726WBL01


Tgt Ion:	96	Resp:	27569
Ion	Ratio	Lower	Upper
96	100		
70	19.1	14.0	21.0
95	9.1	8.7	13.1
97	6.5	0.0	0.0

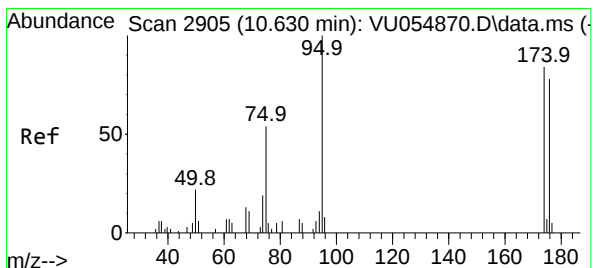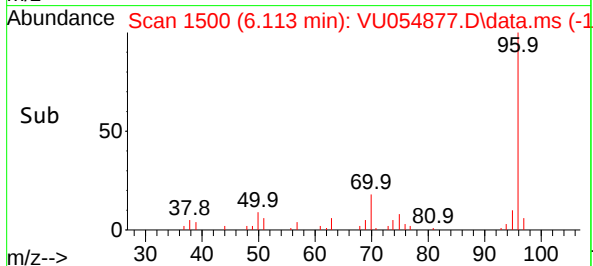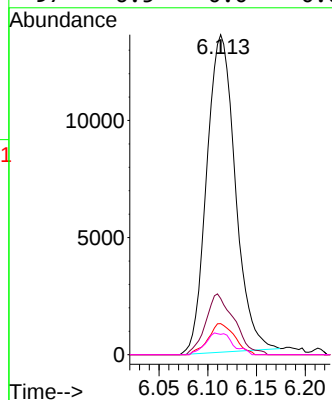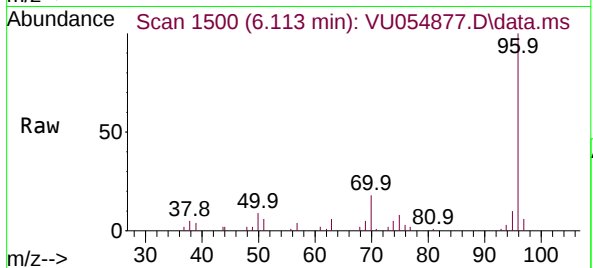

#57
4-Bromofluorobenzene
Concen: 1.000 ug/l
RT: 10.634 min Scan# 2906
Delta R.T. 0.003 min
Lab File: VU054877.D
Acq: 26 Jul 2023 15:37


Tgt Ion:	95	Resp:	8362
Ion	Ratio	Lower	Upper
95	100		
174	94.9	79.3	118.9
176	84.0	71.5	107.3

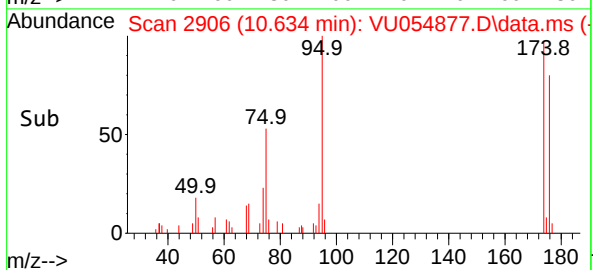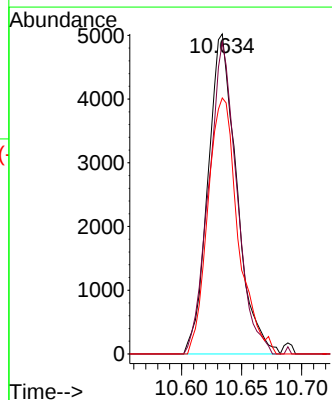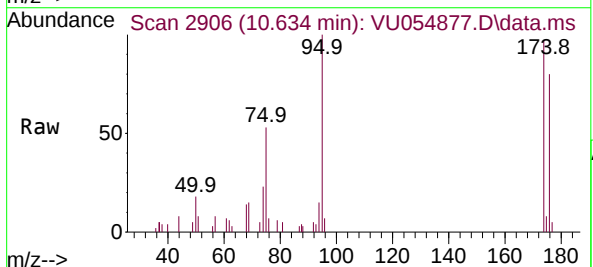

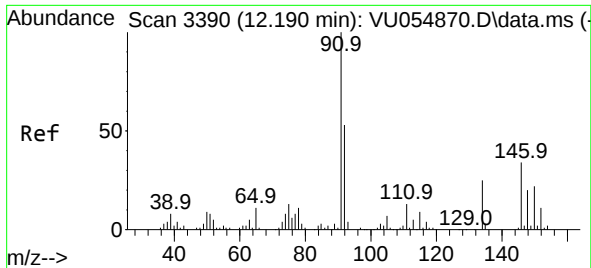

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.961 ug/l
 RT: 12.193 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VU054877.D
 Acq: 26 Jul 2023 15:37

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0726WBL01

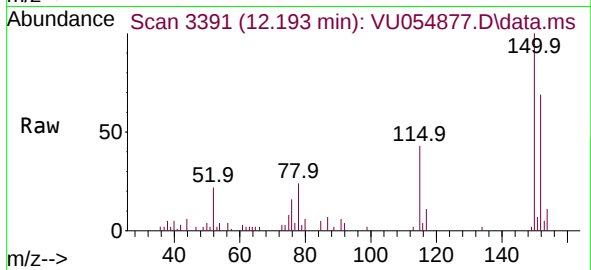

Tgt Ion:	152	Resp:	9079
Ion	Ratio	Lower	Upper
152	100		
115	62.4	0.0	234.8
150	156.4	0.0	598.2

