

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072623\
 Data File : VU054881.D
 Acq On : 26 Jul 2023 17:19
 Operator : MD/SY
 Sample : 03587-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PT-ADD-WS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU054881.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.576	385	400	419	rBV	559596	1030675	44.22%	13.365%
2	3.042	533	545	560	rBV2	24030	45633	1.96%	0.592%
3	3.181	573	588	599	rBV2	16897	38682	1.66%	0.502%
4	3.361	625	644	670	rBV	477195	1108281	47.55%	14.371%
5	3.988	819	839	868	rBV	498271	1287965	55.26%	16.701%
6	4.496	977	997	1018	rBV2	206636	534704	22.94%	6.934%
7	4.640	1027	1042	1059	rBV2	12194	35310	1.51%	0.458%
8	5.936	1427	1445	1465	rBV	533730	1135784	48.73%	14.728%
9	6.113	1488	1500	1514	rVB2	28007	56138	2.41%	0.728%
10	10.634	2895	2906	2922	rVB2	26261	43459	1.86%	0.564%
11	10.904	2976	2990	3014	rBV	1514011	2330861	100.00%	30.225%
12	12.193	3377	3391	3406	rVB3	36326	64277	2.76%	0.833%




Sum of corrected areas: 7711769

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072623\
Data File : VU054881.D
Acq On : 26 Jul 2023 17:19
Operator : MD/SY
Sample : 03587-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-ADD-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

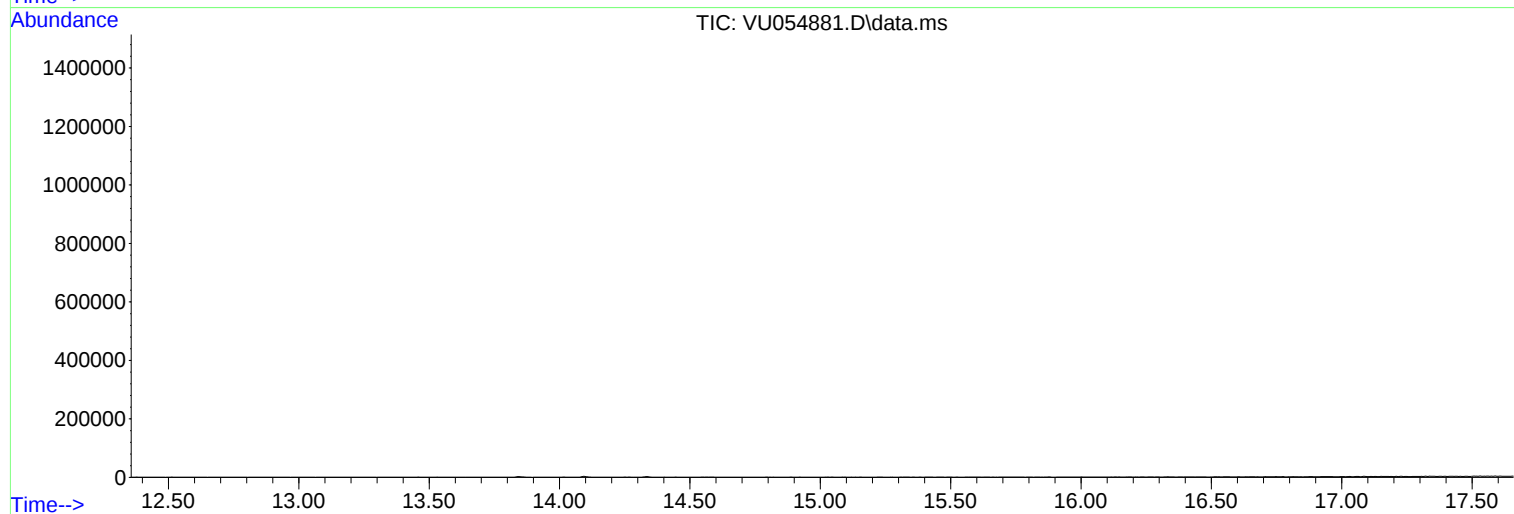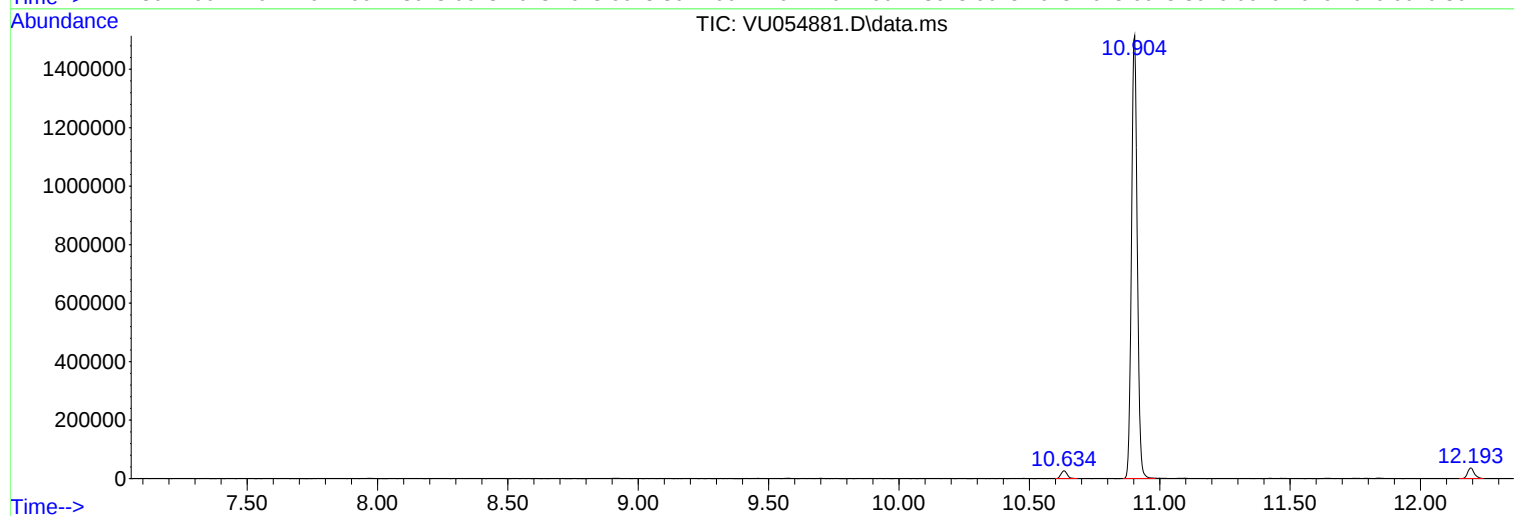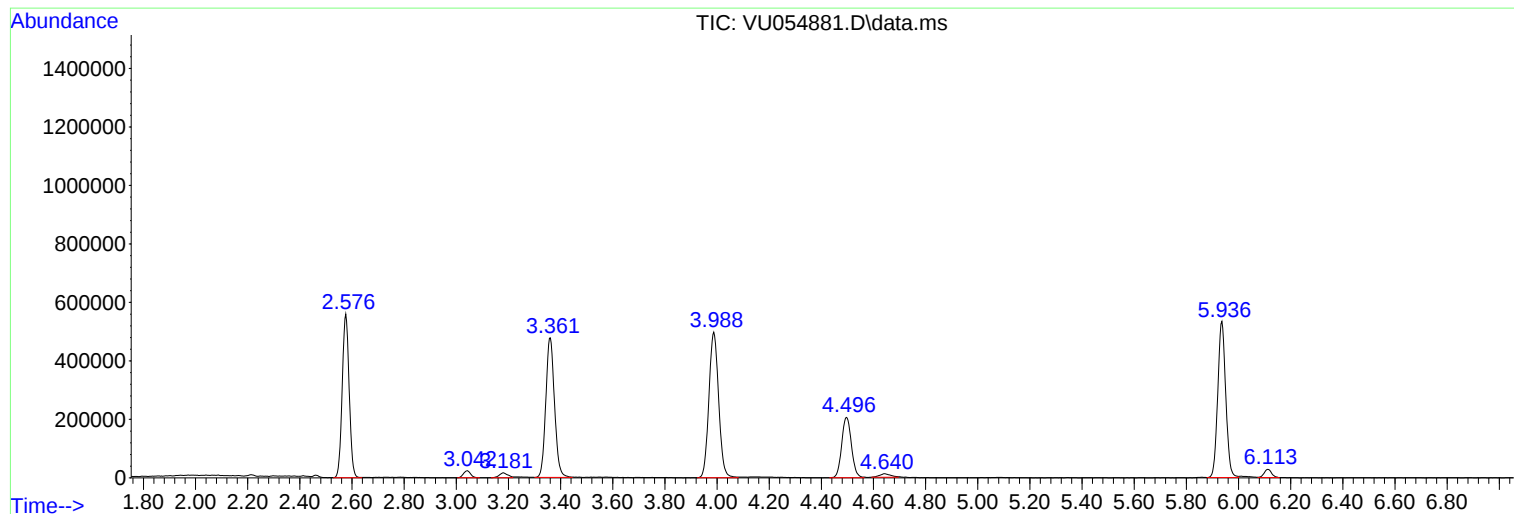

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072623\
Data File : VU054881.D
Acq On : 26 Jul 2023 17:19
Operator : MD/SY
Sample : 03587-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-ADD-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072623\
Data File : VU054881.D
Acq On : 26 Jul 2023 17:19
Operator : MD/SY
Sample : 03587-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-ADD-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc