

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072623\
 Data File : VU054885.D
 Acq On : 26 Jul 2023 18:57
 Operator : MD/SY
 Sample : 03587-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PT-RVOA-WS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU054885.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.576	388	400	414	rVB2	58191	95573	5.51%	0.719%
2	3.039	528	544	570	rBV	217555	406048	23.40%	3.054%
3	3.348	624	640	663	rBV	188644	376438	21.69%	2.831%
4	4.660	1025	1048	1074	rBV2	130575	327266	18.86%	2.461%
5	5.309	1234	1250	1270	rBV2	168069	382693	22.05%	2.878%
6	5.521	1299	1316	1334	rBV	233764	508289	29.29%	3.823%
7	5.772	1376	1394	1415	rBV2	611065	1478212	85.17%	11.118%
8	6.113	1489	1500	1513	rBV2	27379	55050	3.17%	0.414%
9	6.537	1618	1632	1651	rBV	374085	703851	40.55%	5.294%
10	6.788	1697	1710	1727	rBV2	126831	248498	14.32%	1.869%
11	7.965	2062	2076	2107	rBV	509636	886120	51.06%	6.665%
12	8.396	2197	2210	2232	rBV	100838	178754	10.30%	1.344%
13	8.550	2245	2258	2275	rBV2	149707	258858	14.92%	1.947%
14	9.444	2521	2536	2554	rBV	169485	287545	16.57%	2.163%
15	9.566	2561	2574	2599	rBV	942719	1484692	85.55%	11.167%
16	9.688	2599	2612	2650	rVB	728580	1239602	71.42%	9.323%
17	10.100	2726	2740	2765	rBV4	917525	1735548	100.00%	13.053%
18	10.630	2896	2905	2920	rVB3	27000	44833	2.58%	0.337%
19	11.833	3259	3279	3300	rBV	680643	1077700	62.10%	8.106%
20	12.209	3379	3396	3413	rBV2	515810	878721	50.63%	6.609%
21	13.836	3889	3902	3924	rBV	404962	641582	36.97%	4.825%


Sum of corrected areas: 13295873

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072623\
Data File : VU054885.D
Acq On : 26 Jul 2023 18:57
Operator : MD/SY
Sample : 03587-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-RVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

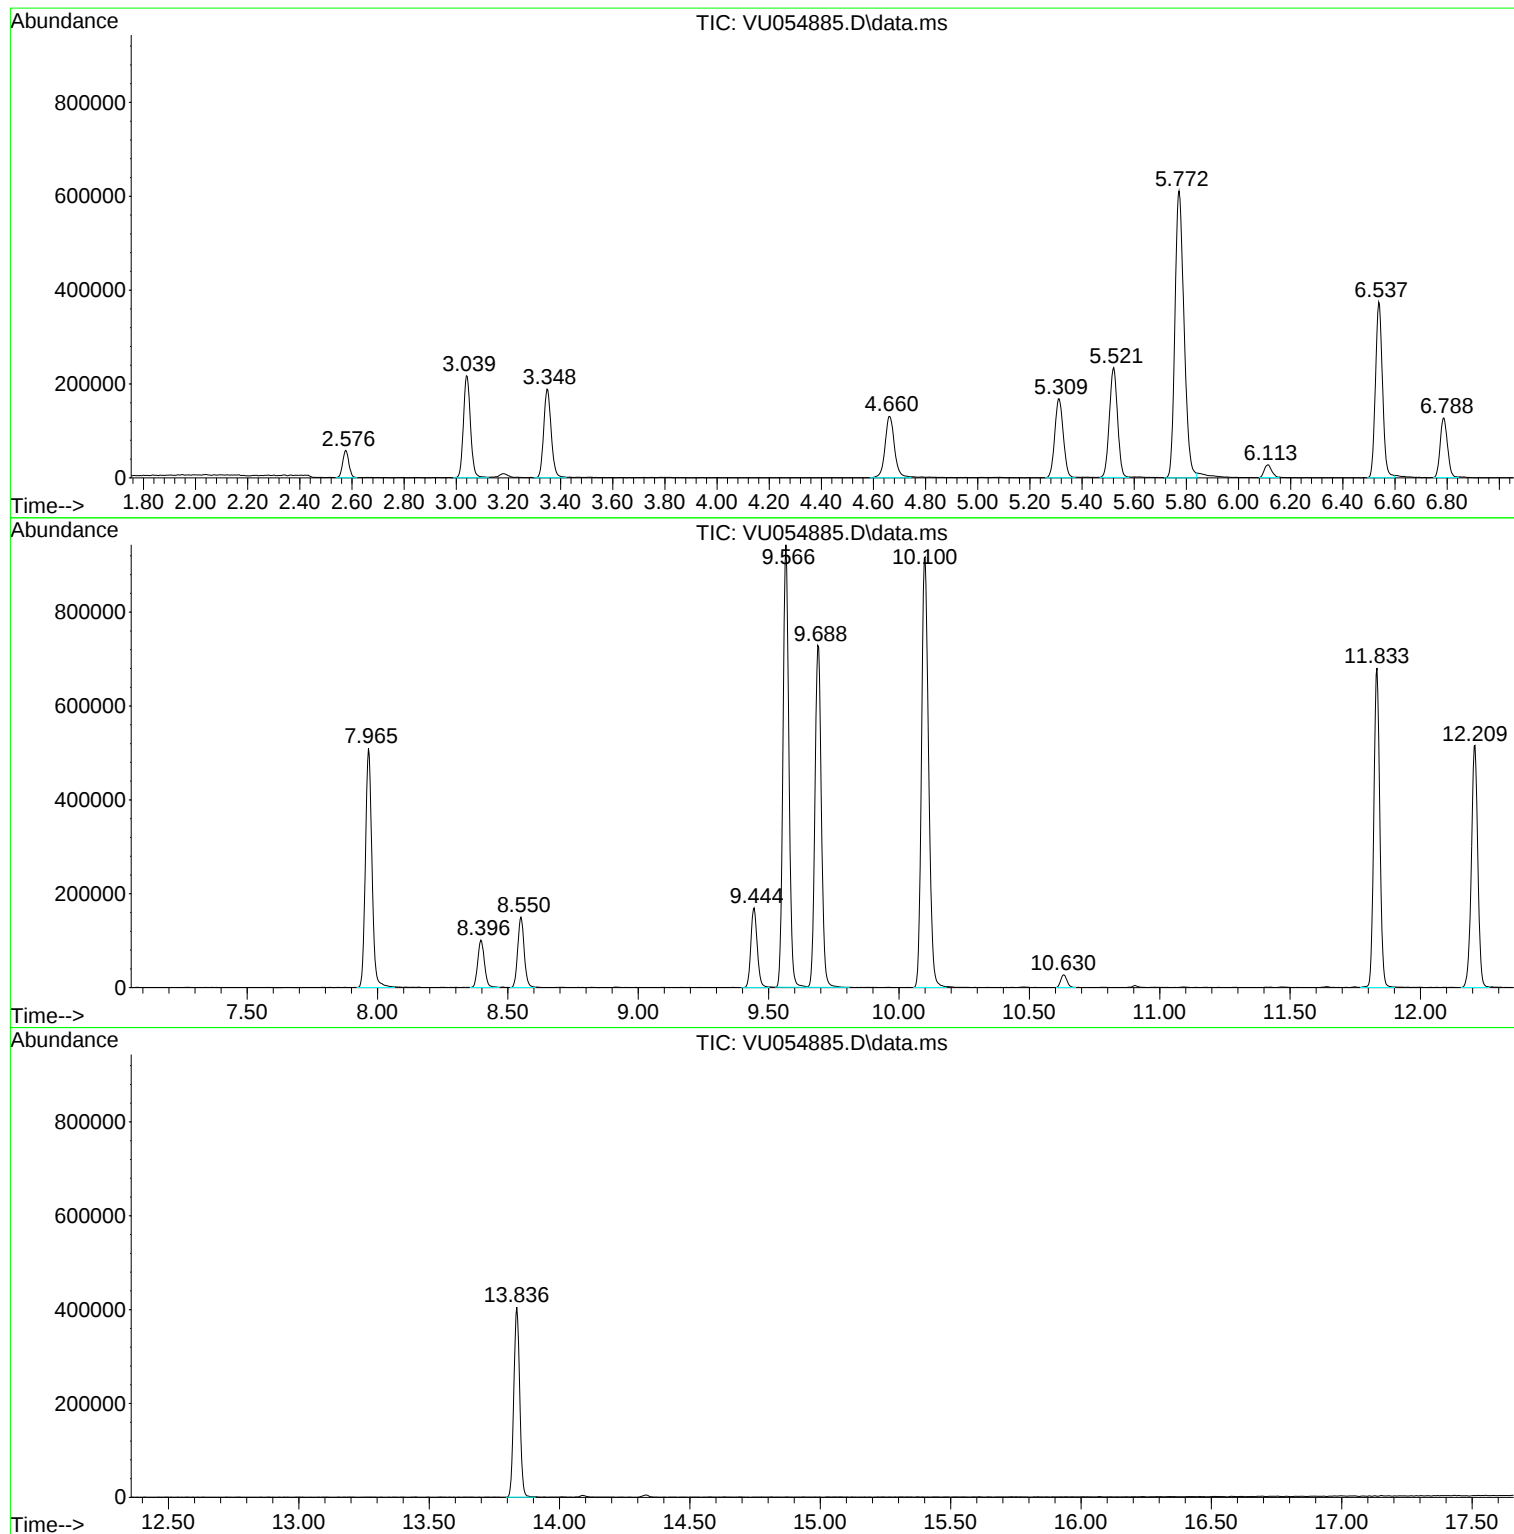

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072623\
Data File : VU054885.D
Acq On : 26 Jul 2023 18:57
Operator : MD/SY
Sample : 03587-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-RVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072623\
Data File : VU054885.D
Acq On : 26 Jul 2023 18:57
Operator : MD/SY
Sample : 03587-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-RVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------