

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072623\
 Data File : VU054887.D
 Acq On : 26 Jul 2023 19:46
 Operator : MD/SY
 Sample : 03587-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PT-UNRVOA-WS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU054887.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.930	190	199	214	rBV	279659	361804	23.50%	1.998%
2	3.042	532	545	560	rBV2	25936	49359	3.21%	0.273%
3	3.361	625	644	669	rBV	620599	1437370	93.37%	7.936%
4	3.866	782	801	825	rBV	204864	485745	31.55%	2.682%
5	4.660	1025	1048	1065	rBV4	66348	181463	11.79%	1.002%
6	4.968	1128	1144	1168	rBV	98745	222329	14.44%	1.228%
7	5.521	1300	1316	1336	rBV	297058	610338	39.65%	3.370%
8	6.113	1488	1500	1516	rBV	28194	54874	3.56%	0.303%
9	6.917	1738	1750	1773	rBV2	69818	134316	8.72%	0.742%
10	7.605	1952	1964	1987	rBV	158577	285707	18.56%	1.577%
11	8.206	2138	2151	2177	rBV2	181857	317563	20.63%	1.753%
12	8.573	2251	2265	2292	rBV	185237	324687	21.09%	1.793%
13	9.531	2551	2563	2581	rBV2	135370	230268	14.96%	1.271%
14	10.479	2845	2858	2880	rBV	864520	1336885	86.84%	7.381%
15	10.631	2892	2905	2920	rBV	29493	45039	2.93%	0.249%
16	10.779	2937	2951	2958	rBV	507291	819337	53.22%	4.524%
17	10.817	2959	2963	2979	rVV2	173214	256120	16.64%	1.414%
18	10.901	2979	2989	3002	rVV	271223	414505	26.93%	2.289%
19	10.981	3002	3014	3031	rVV	577662	925041	60.09%	5.107%
20	11.090	3034	3048	3067	rVB3	797613	1356718	88.13%	7.491%
21	11.415	3133	3149	3156	rBV	578346	889281	57.77%	4.910%
22	11.463	3156	3164	3183	rVB	649581	993940	64.56%	5.488%
23	11.640	3205	3219	3233	rVB	161178	247119	16.05%	1.364%
24	11.743	3238	3251	3258	rBV	757846	1210438	78.63%	6.683%
25	11.788	3258	3265	3277	rVB	579375	872332	56.66%	4.816%
26	12.203	3379	3394	3410	rBV	385127	620591	40.31%	3.426%
27	13.839	3888	3903	3915	rBV8	13136	27955	1.82%	0.154%
28	14.016	3946	3958	3969	rBV	1023192	1537865	99.90%	8.491%
29	14.081	3969	3978	4001	rVB	204238	323535	21.02%	1.786%
30	14.325	4040	4054	4069	rBV	987171	1539463	100.00%	8.500%




Sum of corrected areas: 18111987

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072623\
Data File : VU054887.D
Acq On : 26 Jul 2023 19:46
Operator : MD/SY
Sample : 03587-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-UNRVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

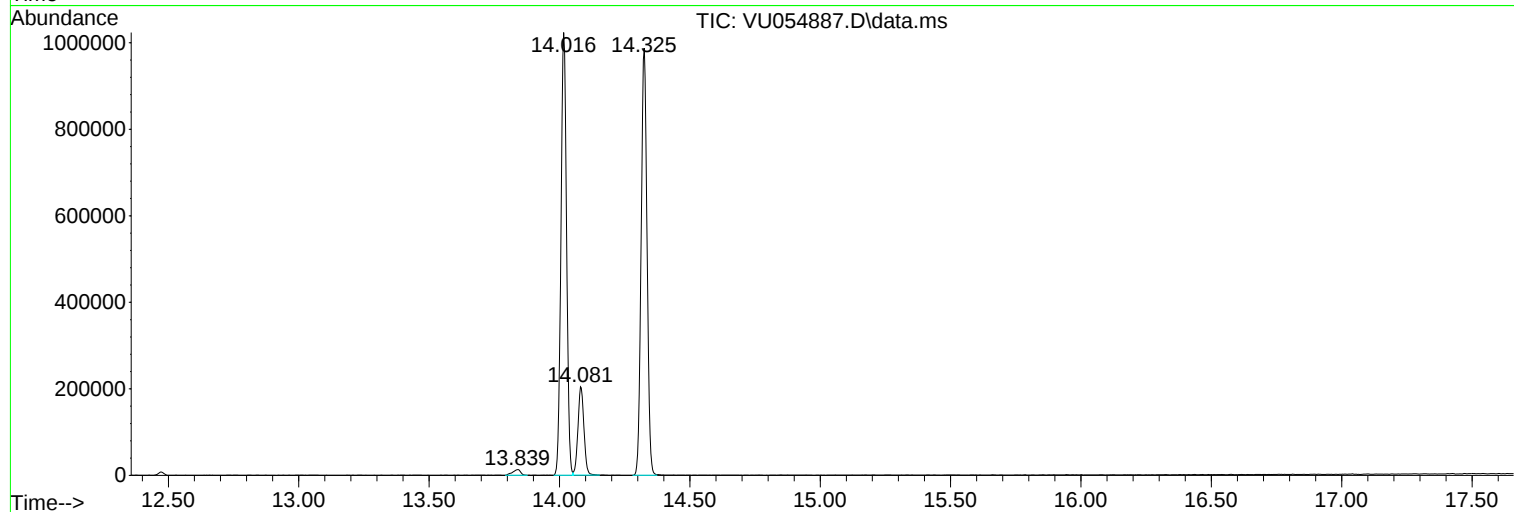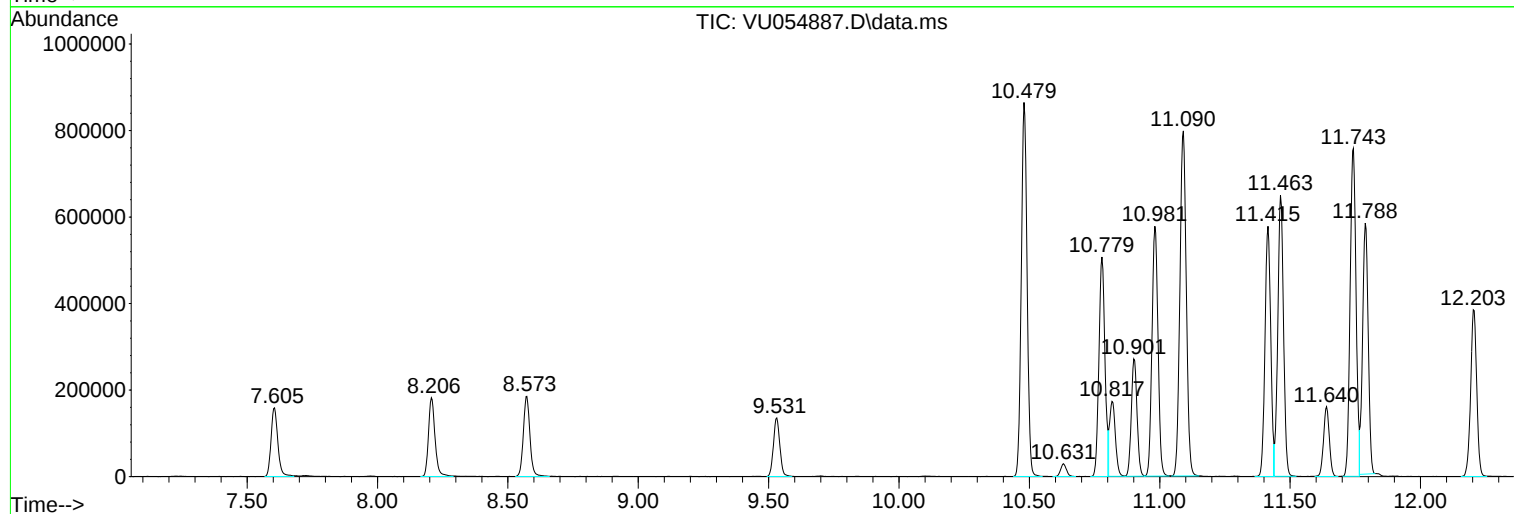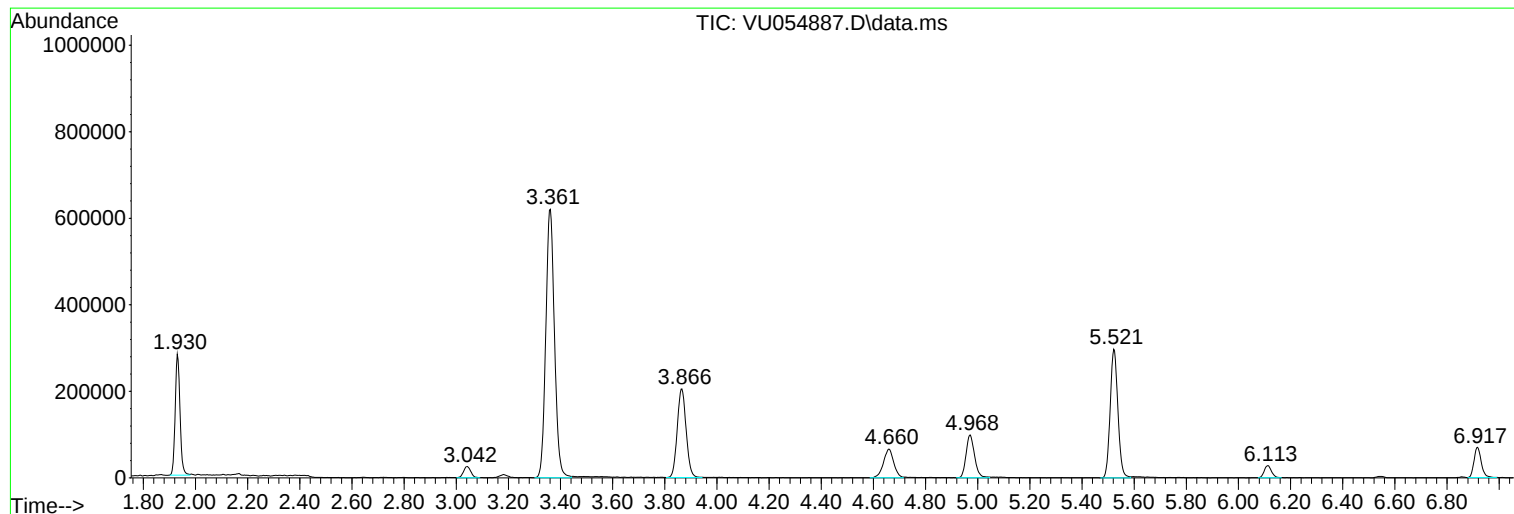

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072623\
Data File : VU054887.D
Acq On : 26 Jul 2023 19:46
Operator : MD/SY
Sample : 03587-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-UNRVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072623\
Data File : VU054887.D
Acq On : 26 Jul 2023 19:46
Operator : MD/SY
Sample : 03587-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-UNRVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------