




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072624\
Data File : VU060236.D
Acq On : 26 Jul 2024 20:12
Operator : MD/SY
Sample : P3359-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G66

Manual IntegrationsAPPROVED

Quant Time: Jul 26 23:19:06 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 26 23:14:26 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

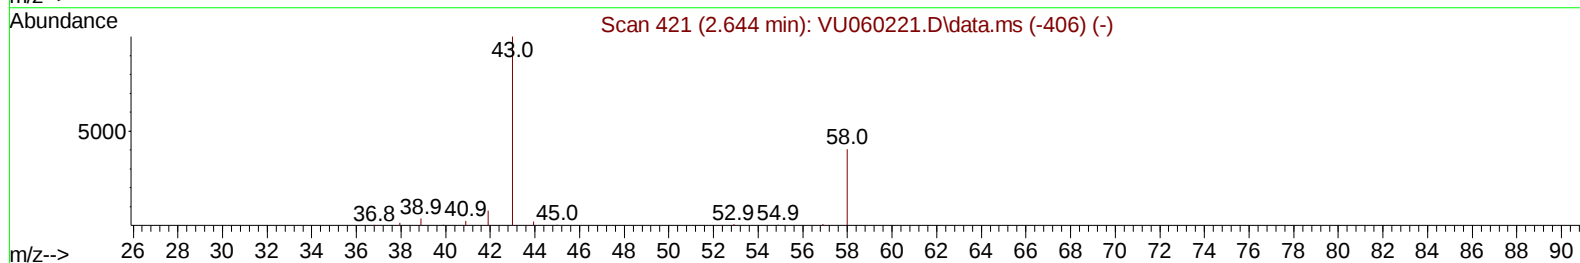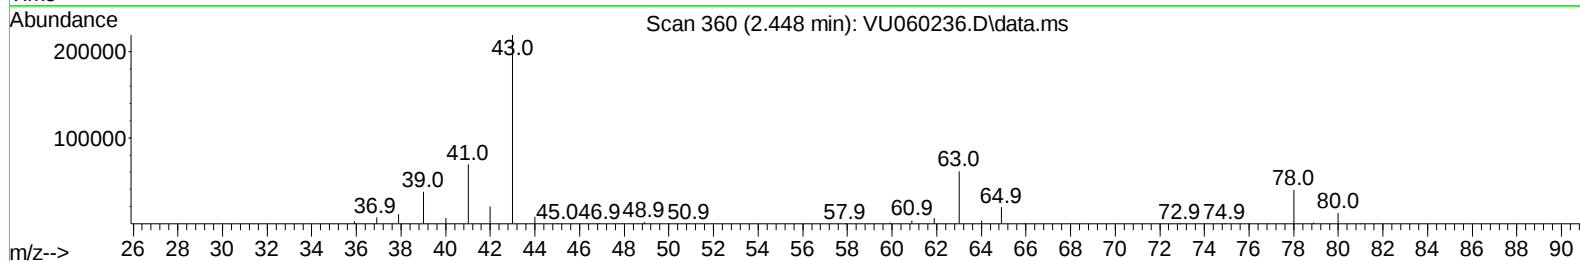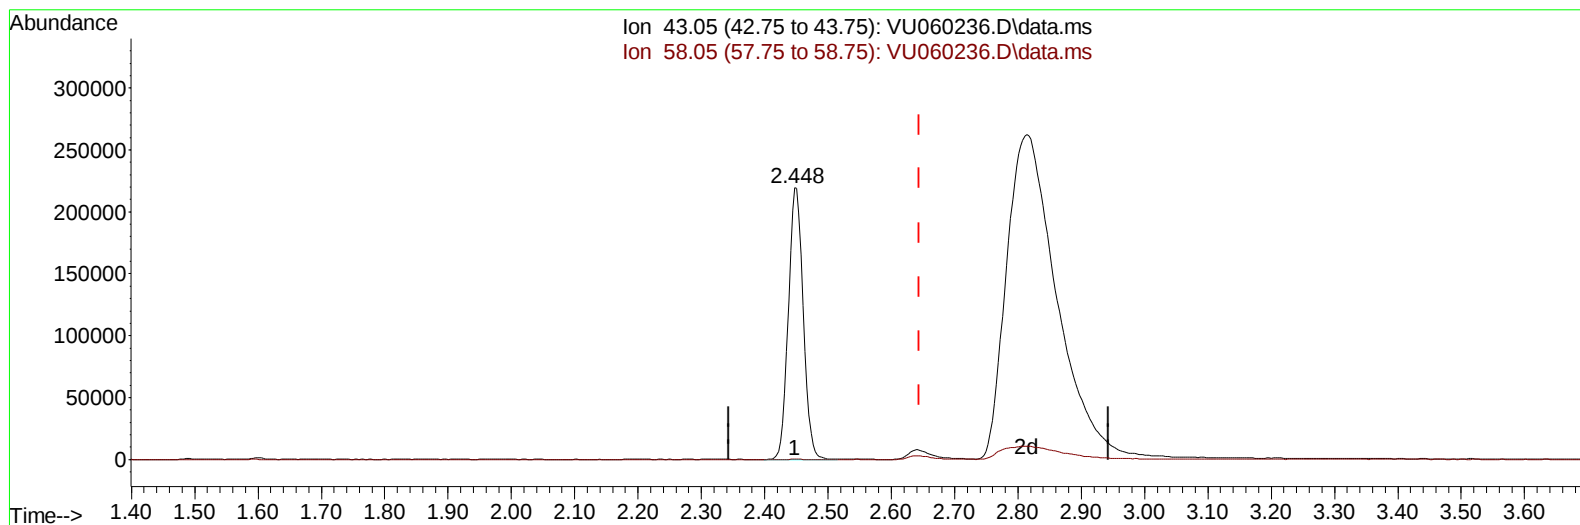

TIC: VU060236.D\data.ms

(13) Acetone (T)

2.448min (-0.196) 252.46 ug/L

response 357898

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.10	2.10
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072624\
Data File : VU060236.D
Acq On : 26 Jul 2024 20:12
Operator : MD/SY
Sample : P3359-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G66

Manual IntegrationsAPPROVED

Quant Time: Jul 26 23:19:06 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 26 23:14:26 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

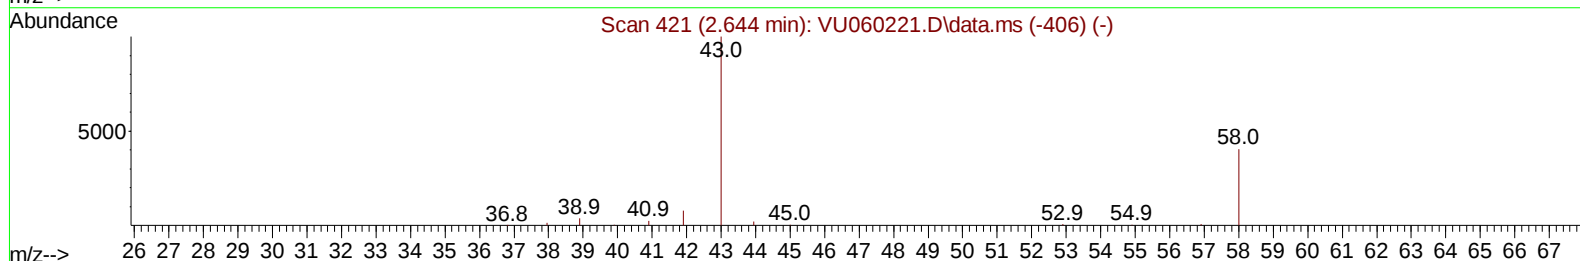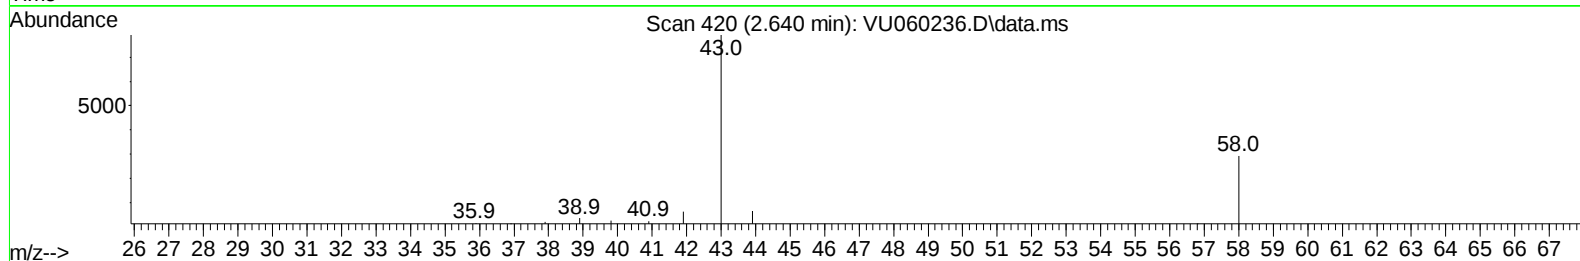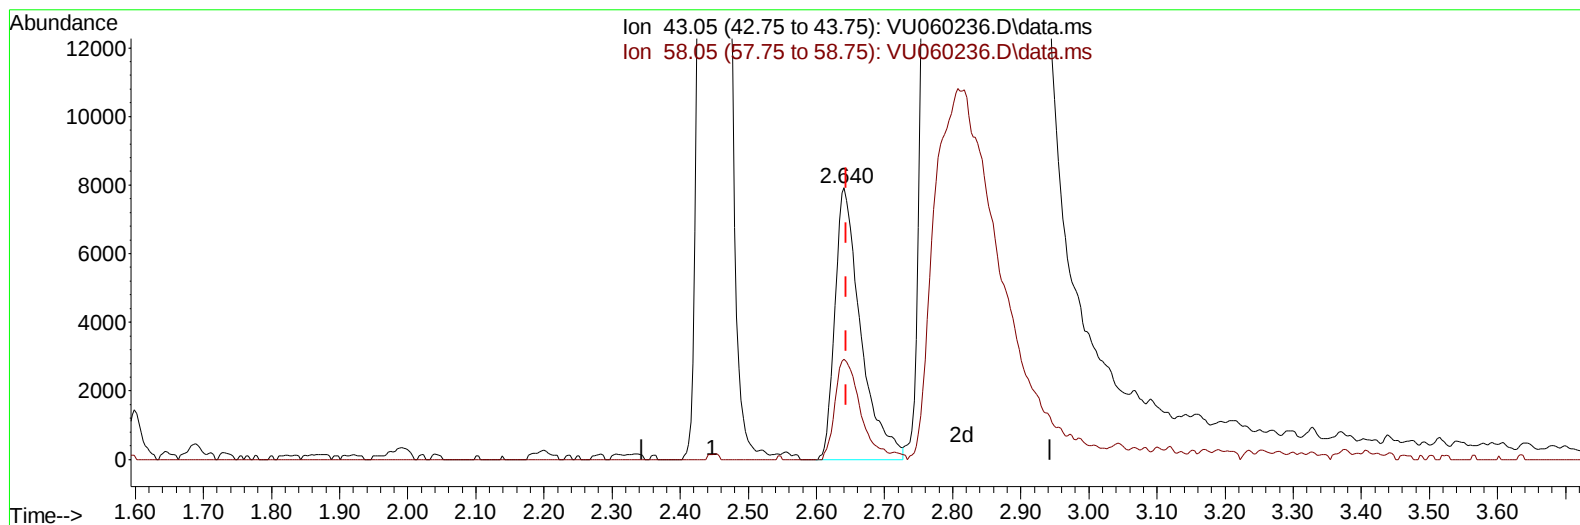

TIC: VU060236.D\data.ms

(13) Acetone (T)

2.640min (-0.003) 14.69 ug/L m

response 20829

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.10	36.09
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072624\
 Data File : VU060236.D
 Acq On : 26 Jul 2024 20:12
 Operator : MD/SY
 Sample : P3359-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1G66

Manual IntegrationsAPPROVED

Quant Time: Jul 26 23:19:06 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jul 26 23:14:26 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/30/2024
 Supervised By :Semsettin Yesilyurt 07/30/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.245	114		131746	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		141490	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		57753	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.595	65		37924	4.137	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	82.800%	
7) Chloroethane-d5	1.911	69		38204	4.486	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	89.800%	
11) 1,1-Dichloroethene-d2	2.560	65		14336	4.006	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	80.200%	
20) 2-Butanone-d5	4.624	46		145469	67.879	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	135.760%#	
24) Chloroform-d	5.055	84		86269	4.478	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	89.600%	
26) 1,2-Dichloroethane-d4	5.695	65		45072	5.025	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	100.400%	
32) Benzene-d6	5.721	84		152105	4.012	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	80.200%	
36) 1,2-Dichloropropane-d6	6.685	67		58270	4.824	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	96.400%	
41) Toluene-d8	7.894	98		112876	3.295	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	66.000%#	
43) trans-1,3-Dichloroprop...	8.177	79		17183	4.179	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	83.600%	
46) 2-Hexanone-d5	8.627	63		96085	52.658	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	105.320%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84		54407	5.061	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	101.200%	
66) 1,2-Dichlorobenzene-d4	12.190	152		49001	4.701	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	94.000%	
Target Compounds							
2) Dichlorodifluoromethane	1.383	85		24305	2.440	ug/L	100
13) Acetone	2.640	43		20829m	14.693	ug/L	
42) Toluene	7.968	91		16287	0.327	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072624\
Data File : VU060236.D
Acq On : 26 Jul 2024 20:12
Operator : MD/SY
Sample : P3359-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G66

Manual IntegrationsAPPROVED

Quant Time: Jul 26 23:19:06 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 26 23:14:26 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

