




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072624\
Data File : VU060237.D
Acq On : 26 Jul 2024 20:36
Operator : MD/SY
Sample : P3359-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G76

Manual IntegrationsAPPROVED

Quant Time: Jul 26 23:19:23 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 26 23:14:26 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

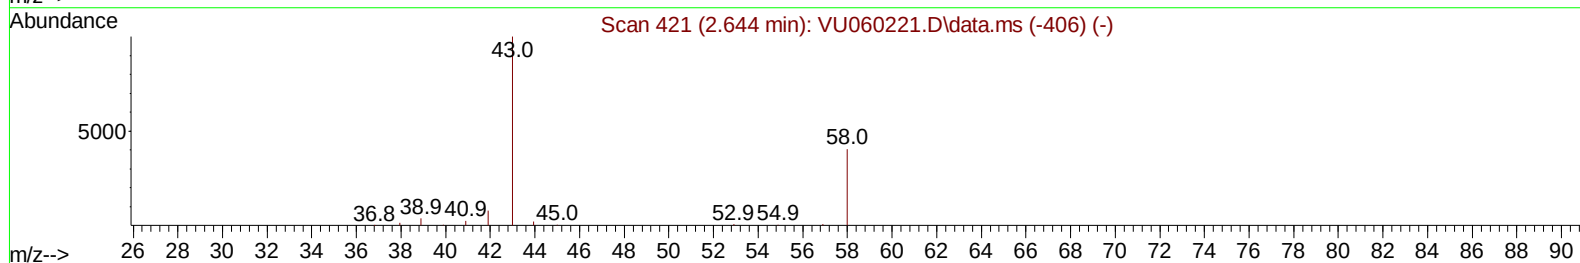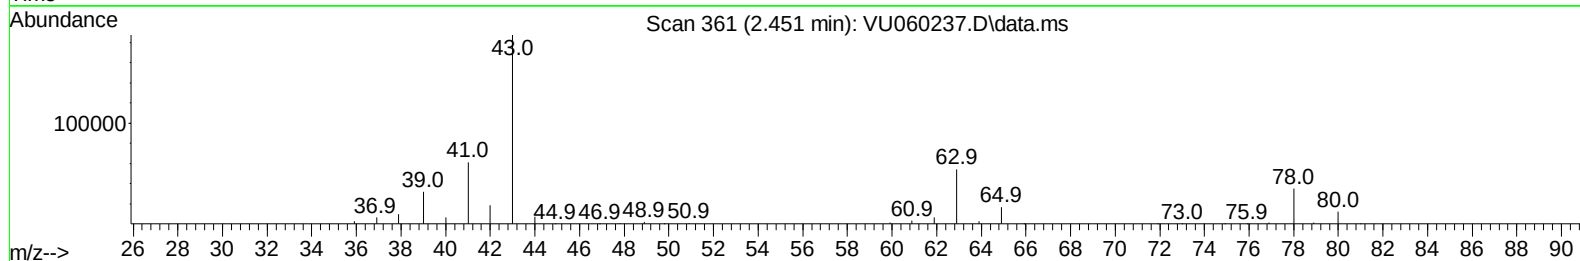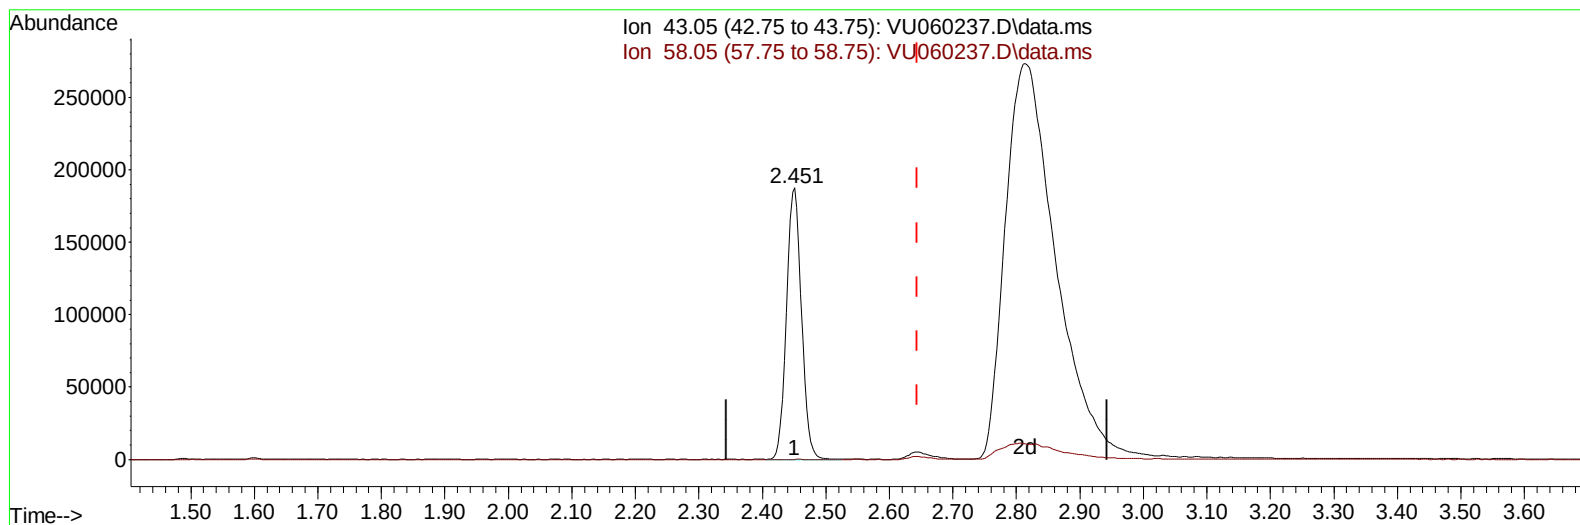

TIC: VU060237.D\data.ms

(13) Acetone (T)

2.451min (-0.193) 221.34 ug/L

response 305997

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.10	1.49
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072624\
Data File : VU060237.D
Acq On : 26 Jul 2024 20:36
Operator : MD/SY
Sample : P3359-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G76

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

Quant Time: Jul 26 23:19:23 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 26 23:14:26 2024
Response via : Initial Calibration

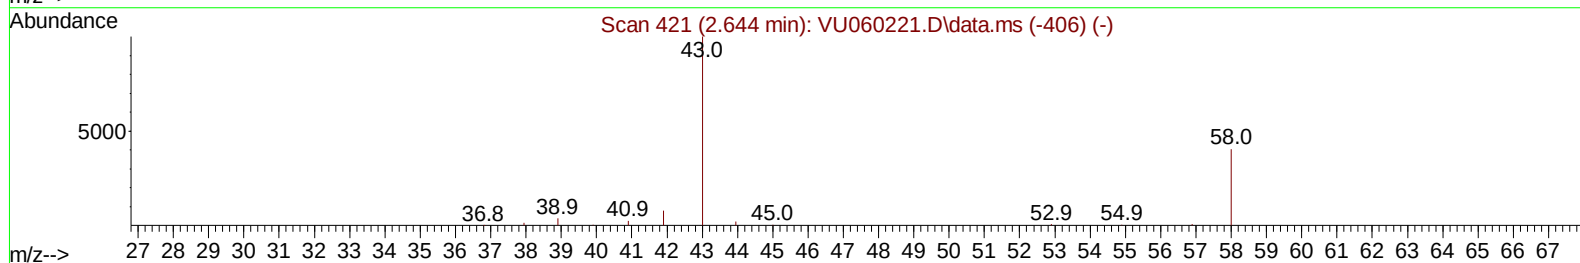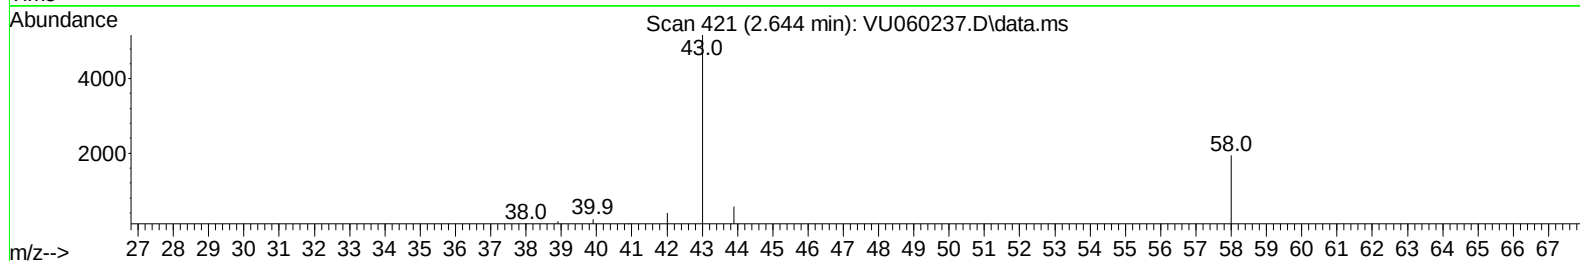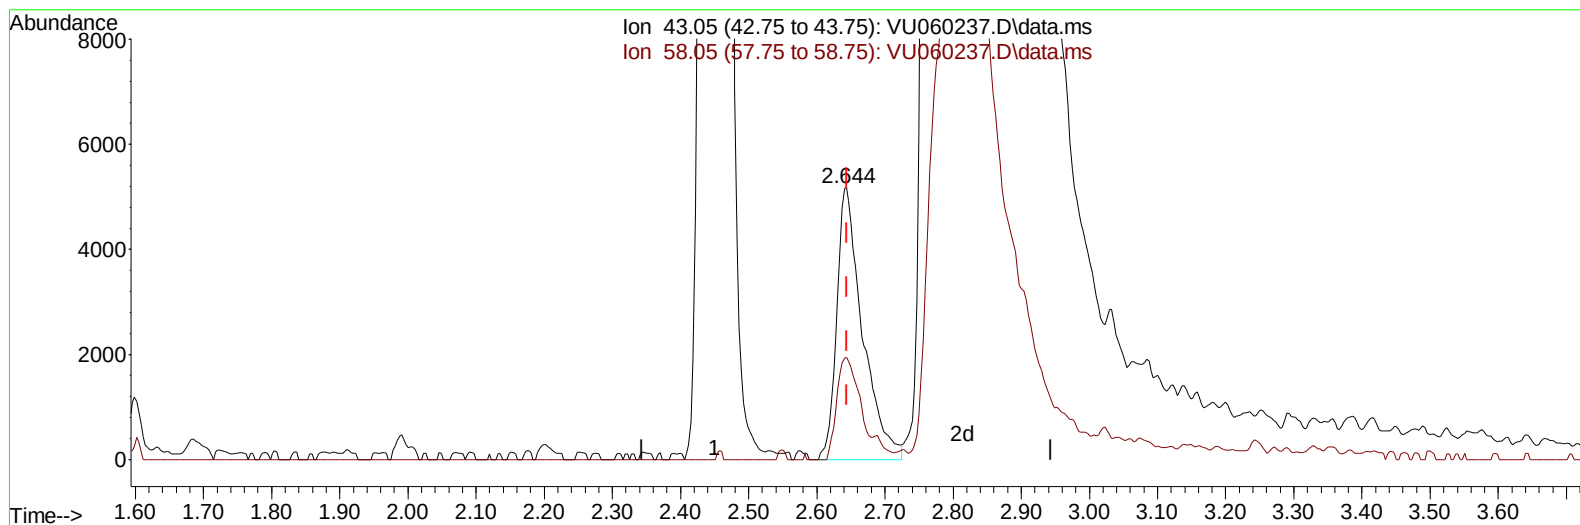

TIC: VU060237.D\data.ms

(13) Acetone (T)

2.644min (-0.000) 9.82 ug/L m

response 13579

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.10	33.55
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072624\
 Data File : VU060237.D
 Acq On : 26 Jul 2024 20:36
 Operator : MD/SY
 Sample : P3359-09
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1G76

Manual IntegrationsAPPROVED

Quant Time: Jul 26 23:19:23 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jul 26 23:14:26 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/30/2024
 Supervised By :Semsettin Yesilyurt 07/30/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.245	114		128482	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		136972	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		55471	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.595	65		35525	3.974	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	79.400%	
7) Chloroethane-d5	1.911	69		35535	4.279	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	85.600%	
11) 1,1-Dichloroethene-d2	2.563	65		13769	3.945	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	79.000%	
20) 2-Butanone-d5	4.624	46		136676	65.396	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	130.800%#	
24) Chloroform-d	5.058	84		82018	4.366	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	87.400%	
26) 1,2-Dichloroethane-d4	5.698	65		41914	4.791	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	95.800%	
32) Benzene-d6	5.721	84		145154	3.955	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	79.200%	
36) 1,2-Dichloropropane-d6	6.685	67		55934	4.783	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	95.600%	
41) Toluene-d8	7.894	98		105004	3.167	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	63.400%#	
43) trans-1,3-Dichloroprop...	8.177	79		16415	4.124	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	82.400%	
46) 2-Hexanone-d5	8.627	63		88178	49.919	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	99.840%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84		52385	5.033	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	100.600%	
66) 1,2-Dichlorobenzene-d4	12.190	152		48039	4.798	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	96.000%	
Target Compounds							
2) Dichlorodifluoromethane	1.383	85		23361	2.405	ug/L	99
13) Acetone	2.644	43		13579m	9.822	ug/L	
42) Toluene	7.968	91		18685	0.388	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072624\
Data File : VU060237.D
Acq On : 26 Jul 2024 20:36
Operator : MD/SY
Sample : P3359-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G76

Manual IntegrationsAPPROVED

Quant Time: Jul 26 23:19:23 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 26 23:14:26 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

