




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072624\
Data File : VU060238.D
Acq On : 26 Jul 2024 21:00
Operator : MD/SY
Sample : P3359-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G77

Manual IntegrationsAPPROVED

Quant Time: Jul 26 23:19:36 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 26 23:14:26 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

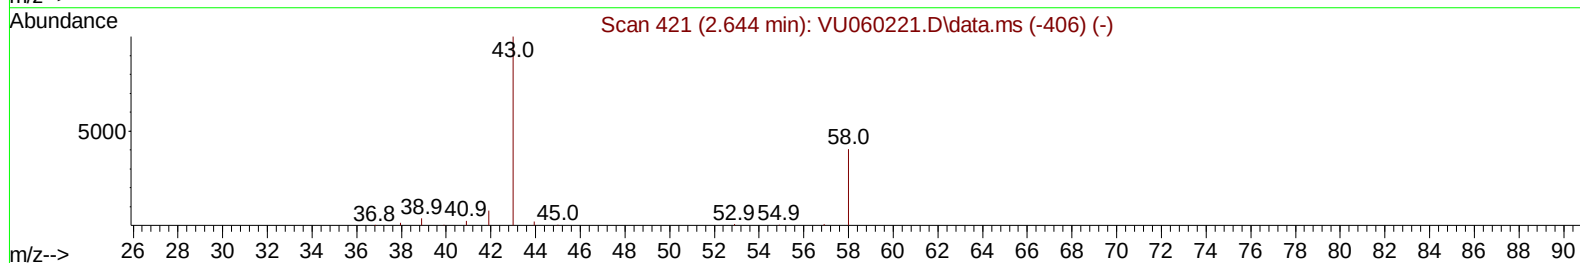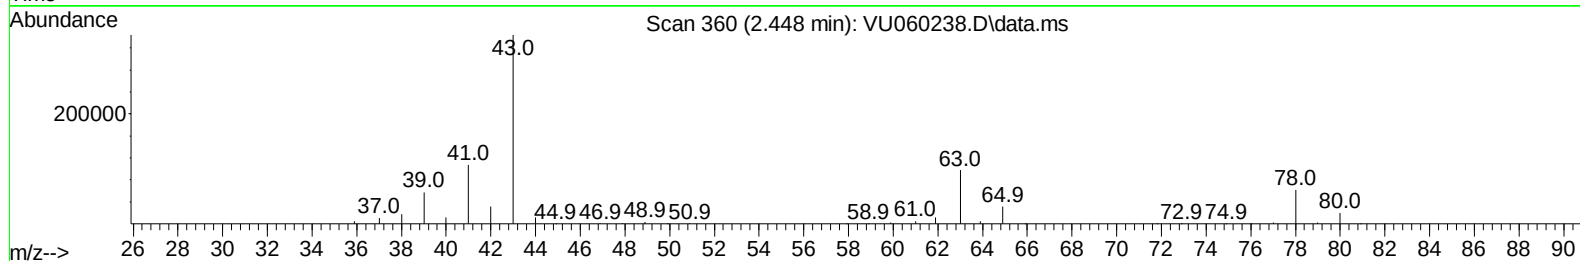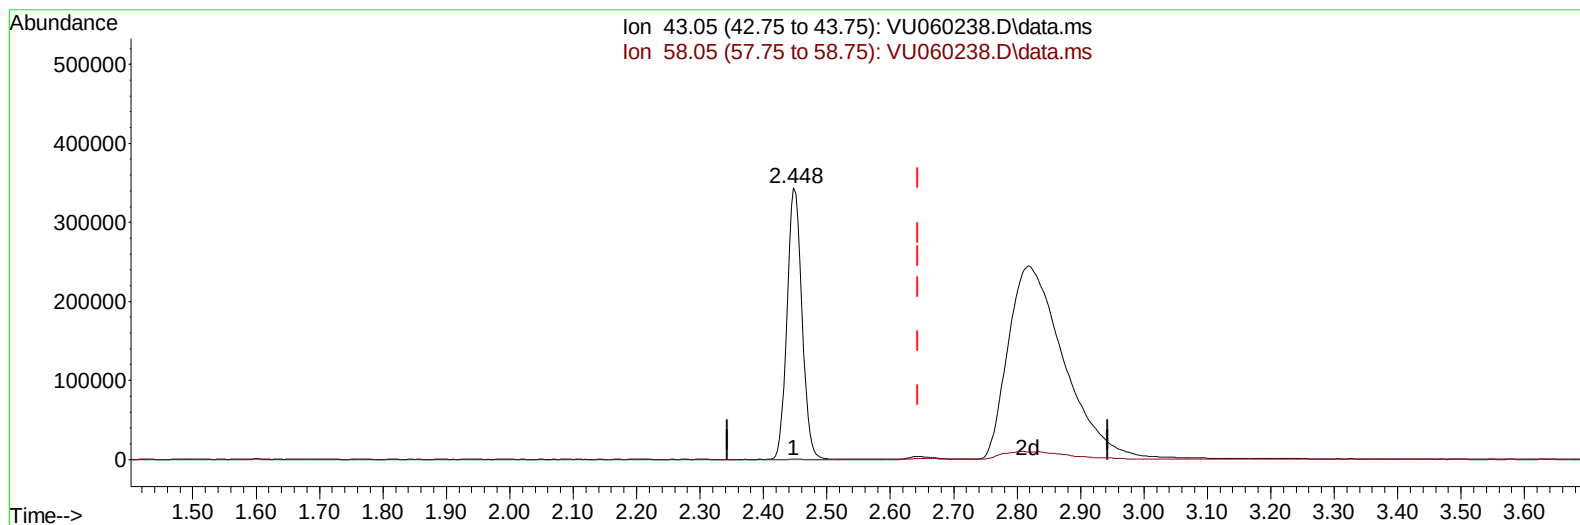

TIC: VU060238.D\data.ms

(13) Acetone (T)

2.448min (-0.196) 382.35 ug/L

response 561845

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.10	0.77
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072624\
Data File : VU060238.D
Acq On : 26 Jul 2024 21:00
Operator : MD/SY
Sample : P3359-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G77

Manual IntegrationsAPPROVED

Quant Time: Jul 26 23:19:36 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 26 23:14:26 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

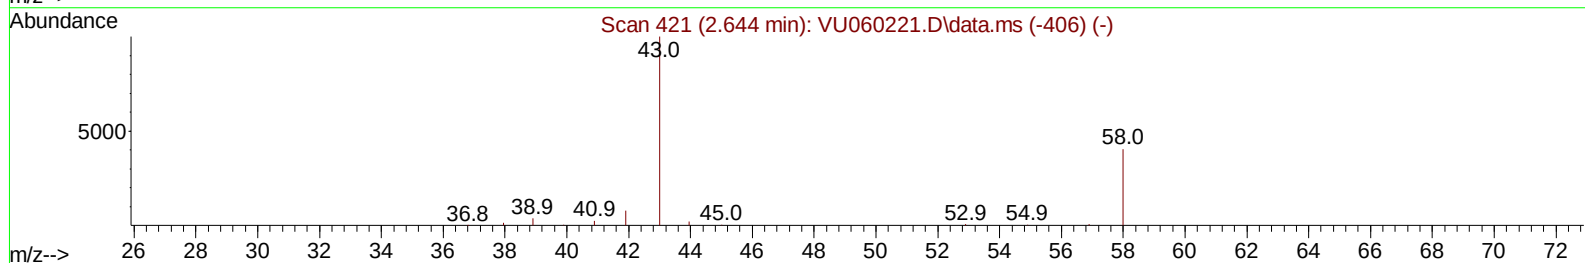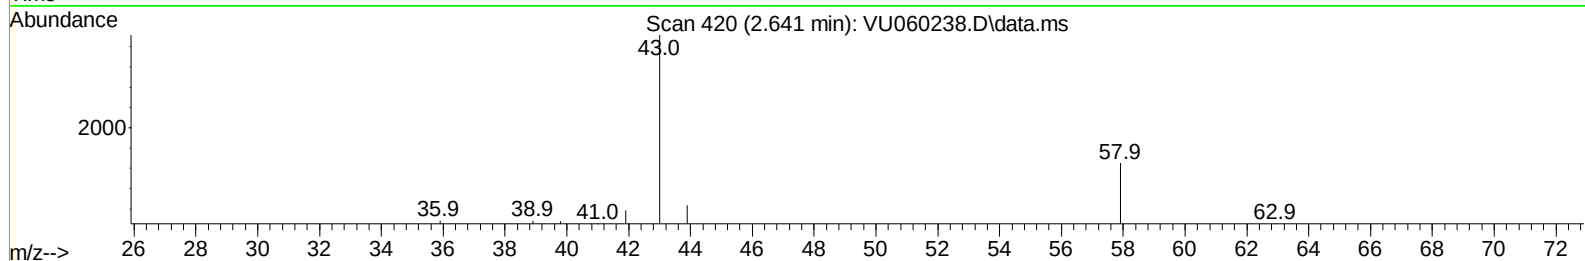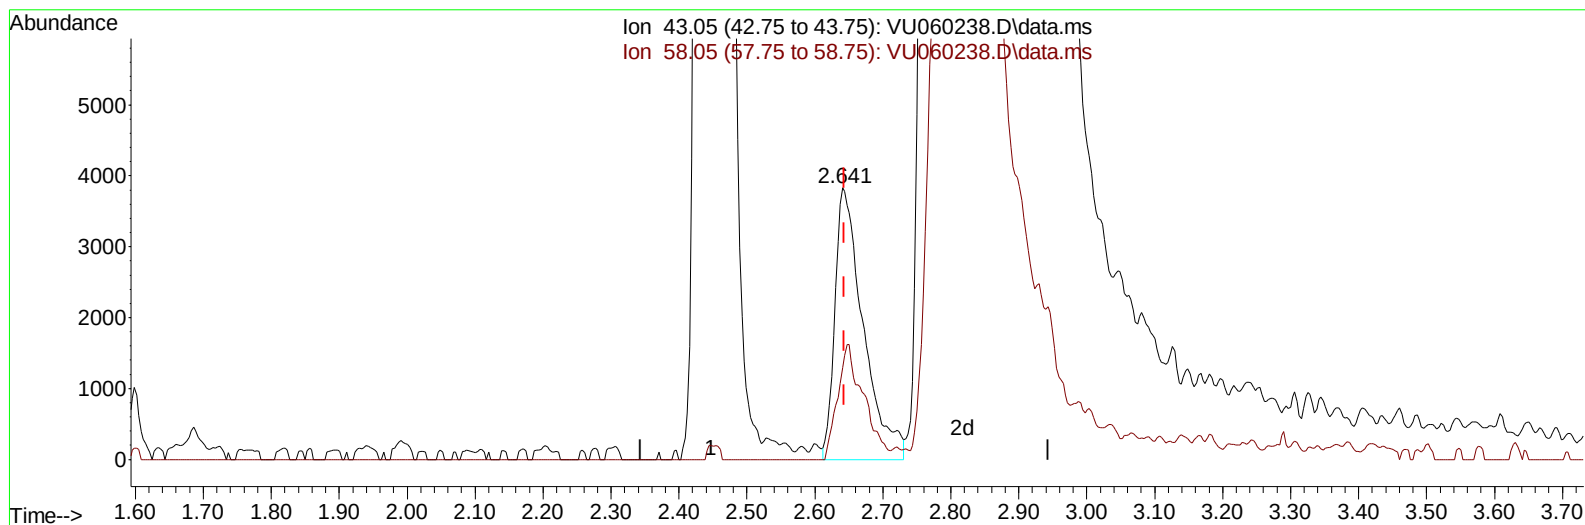

TIC: VU060238.D\data.ms

(13) Acetone (T)

2.641min (-0.003) 7.52 ug/L m

response 11057

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.10	39.09
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072624\
 Data File : VU060238.D
 Acq On : 26 Jul 2024 21:00
 Operator : MD/SY
 Sample : P3359-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1G77

Manual IntegrationsAPPROVED

Quant Time: Jul 26 23:19:36 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jul 26 23:14:26 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/30/2024
 Supervised By :Semsettin Yesilyurt 07/30/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.245	114		136564	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		147465	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152		58381	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.596	65		35184	3.703	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	74.000%	
7) Chloroethane-d5	1.911	69		36044	4.083	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	81.600%	
11) 1,1-Dichloroethene-d2	2.563	65		13202	3.559	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	71.200%	
20) 2-Butanone-d5	4.624	46		131473	59.184	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	118.360%	
24) Chloroform-d	5.055	84		82885	4.151	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	83.000%	
26) 1,2-Dichloroethane-d4	5.695	65		40913	4.400	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	88.000%	
32) Benzene-d6	5.721	84		145481	3.682	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	73.600%	
36) 1,2-Dichloropropane-d6	6.682	67		54536	4.332	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	86.600%	
41) Toluene-d8	7.894	98		106494	2.983	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	59.600%#	
43) trans-1,3-Dichloroprop...	8.177	79		16054	3.746	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	75.000%	
46) 2-Hexanone-d5	8.627	63		89030	46.815	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	93.640%	
56) 1,1,2,2-Tetrachloroeth...	10.750	84		51708	4.615	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	92.200%	
66) 1,2-Dichlorobenzene-d4	12.190	152		47212	4.480	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	89.600%	
Target Compounds							
13) Acetone	2.641	43		11057m	7.524	ug/L	
42) Toluene	7.965	91		47610	0.918	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072624\
Data File : VU060238.D
Acq On : 26 Jul 2024 21:00
Operator : MD/SY
Sample : P3359-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G77

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

Quant Time: Jul 26 23:19:36 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 26 23:14:26 2024
Response via : Initial Calibration

