




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072624\
Data File : VU060239.D
Acq On : 26 Jul 2024 21:24
Operator : MD/SY
Sample : P3359-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GC0

Manual IntegrationsAPPROVED

Quant Time: Jul 26 23:19:53 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 26 23:14:26 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

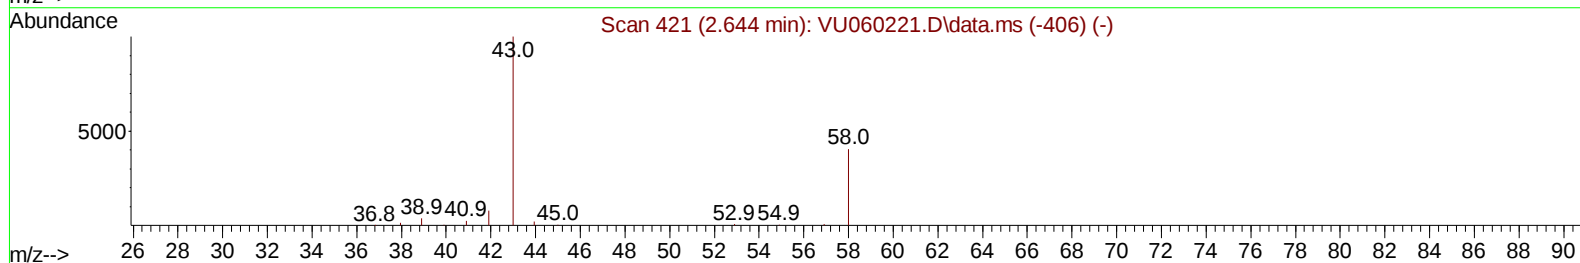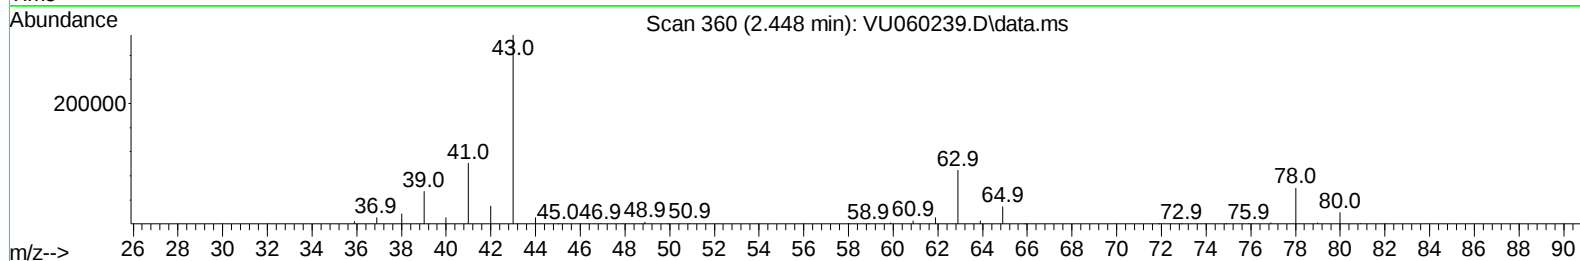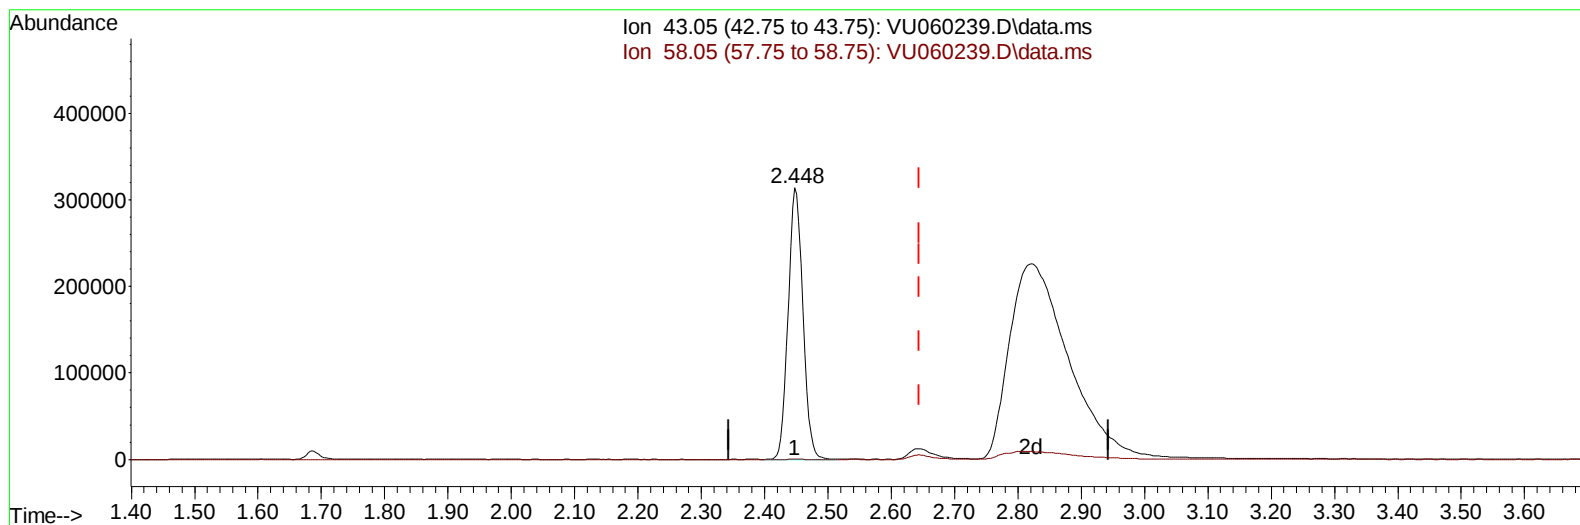

TIC: VU060239.D\data.ms

(13) Acetone (T)

2.448min (-0.196) 364.83 ug/L

response 509514

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.10	2.68
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072624\
Data File : VU060239.D
Acq On : 26 Jul 2024 21:24
Operator : MD/SY
Sample : P3359-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GC0

Manual IntegrationsAPPROVED

Quant Time: Jul 26 23:19:53 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 26 23:14:26 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

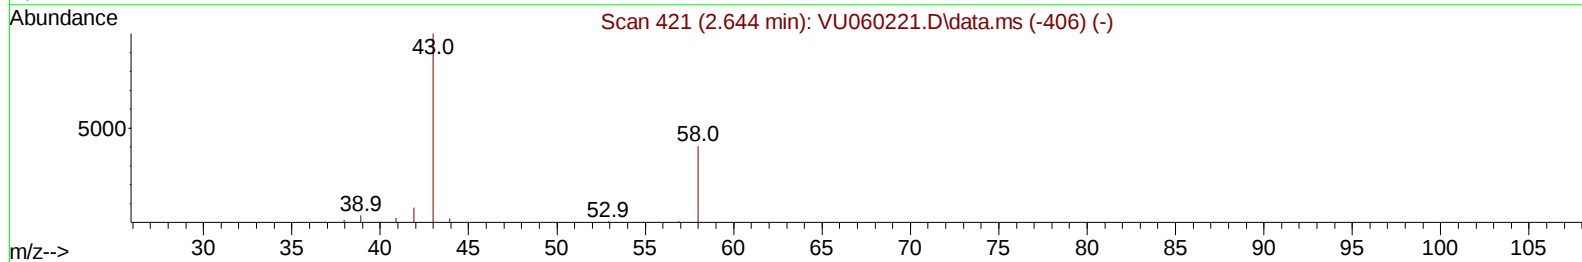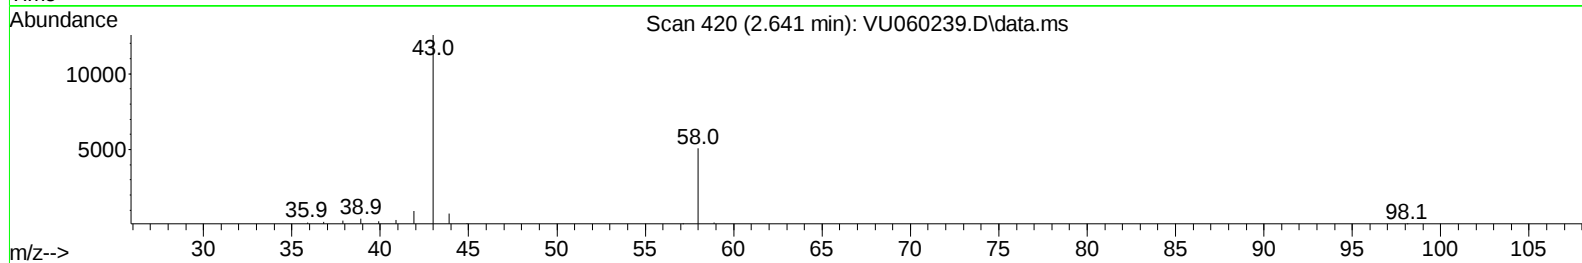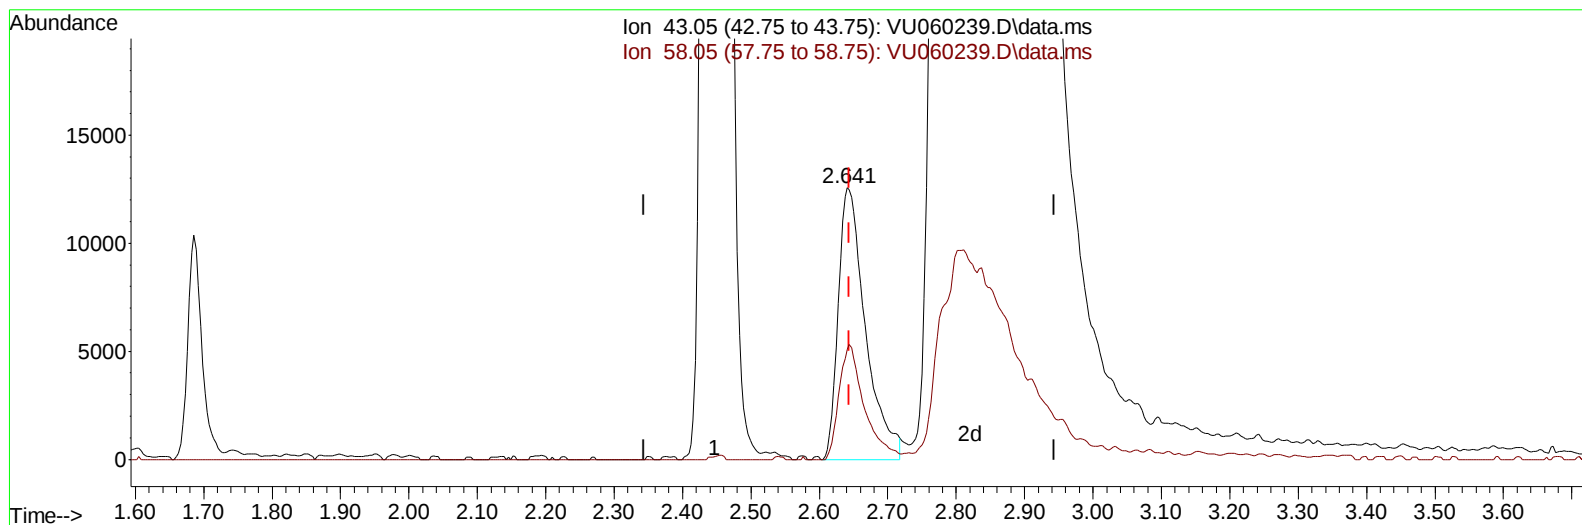

TIC: VU060239.D\data.ms

(13) Acetone (T)

2.641min (-0.003) 24.82 ug/L m

response 34660

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	41.10	39.43
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072624\
 Data File : VU060239.D
 Acq On : 26 Jul 2024 21:24
 Operator : MD/SY
 Sample : P3359-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GC0

Manual IntegrationsAPPROVED

Quant Time: Jul 26 23:19:53 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jul 26 23:14:26 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/30/2024
 Supervised By :Semsettin Yesilyurt 07/30/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.245	114		129791	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		139398	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		56521	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.596	65		36522	4.044	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.800%	
7) Chloroethane-d5	1.908	69		37520	4.472	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.400%	
11) 1,1-Dichloroethene-d2	2.560	65		13688	3.882	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.600%	
20) 2-Butanone-d5	4.628	46		137453	65.105	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	130.200%#	
24) Chloroform-d	5.055	84		86611	4.564	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.200%	
26) 1,2-Dichloroethane-d4	5.695	65		43514	4.924	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.400%	
32) Benzene-d6	5.721	84		152201	4.075	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.600%	
36) 1,2-Dichloropropane-d6	6.685	67		58258	4.895	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.000%	
41) Toluene-d8	7.894	98		112765	3.342	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	66.800%#	
43) trans-1,3-Dichloroprop...	8.177	79		16415	4.052	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.000%	
46) 2-Hexanone-d5	8.627	63		91739	51.031	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.060%	
56) 1,1,2,2-Tetrachloroeth...	10.750	84		54441	5.140	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.800%	
66) 1,2-Dichlorobenzene-d4	12.187	152		52741	5.170	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.400%	
Target Compounds							
13) Acetone	2.641	43		34660m	24.818	ug/L	
16) Methylene chloride	3.046	84		2555	0.210	ug/L	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072624\
Data File : VU060239.D
Acq On : 26 Jul 2024 21:24
Operator : MD/SY
Sample : P3359-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GC0

Manual IntegrationsAPPROVED

Quant Time: Jul 26 23:19:53 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 26 23:14:26 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

