

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072624\
 Data File : VU060229.D
 Acq On : 26 Jul 2024 17:24
 Operator : MD/SY
 Sample : P3244-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Quant Time: Jul 26 23:17:25 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jul 26 23:14:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	138117	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	146175	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	60062	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	38842	4.042	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.800%
7) Chloroethane-d5	1.911	69	37812	4.235	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	84.800%
11) 1,1-Dichloroethene-d2	2.560	65	15062	4.014	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	80.200%
20) 2-Butanone-d5	4.631	46	141365	62.922	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	125.840%
24) Chloroform-d	5.055	84	88853	4.399	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.000%
26) 1,2-Dichloroethane-d4	5.698	65	45204	4.807	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.200%
32) Benzene-d6	5.721	84	156428	3.994	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	79.800%
36) 1,2-Dichloropropane-d6	6.685	67	59871	4.797	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.000%
41) Toluene-d8	7.894	98	117526	3.321	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	66.400%#
43) trans-1,3-Dichloroprop...	8.177	79	17744	4.177	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.600%
46) 2-Hexanone-d5	8.630	63	95994	50.922	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.840%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	54559	4.912	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.200%
66) 1,2-Dichlorobenzene-d4	12.190	152	51487	4.749	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.000%
Target Compounds						Qvalue
16) Methylene chloride	3.042	84	4898	0.379	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072624\
Data File : VU060229.D
Acq On : 26 Jul 2024 17:24
Operator : MD/SY
Sample : P3244-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001


Quant Time: Jul 26 23:17:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 26 23:14:26 2024
Response via : Initial Calibration

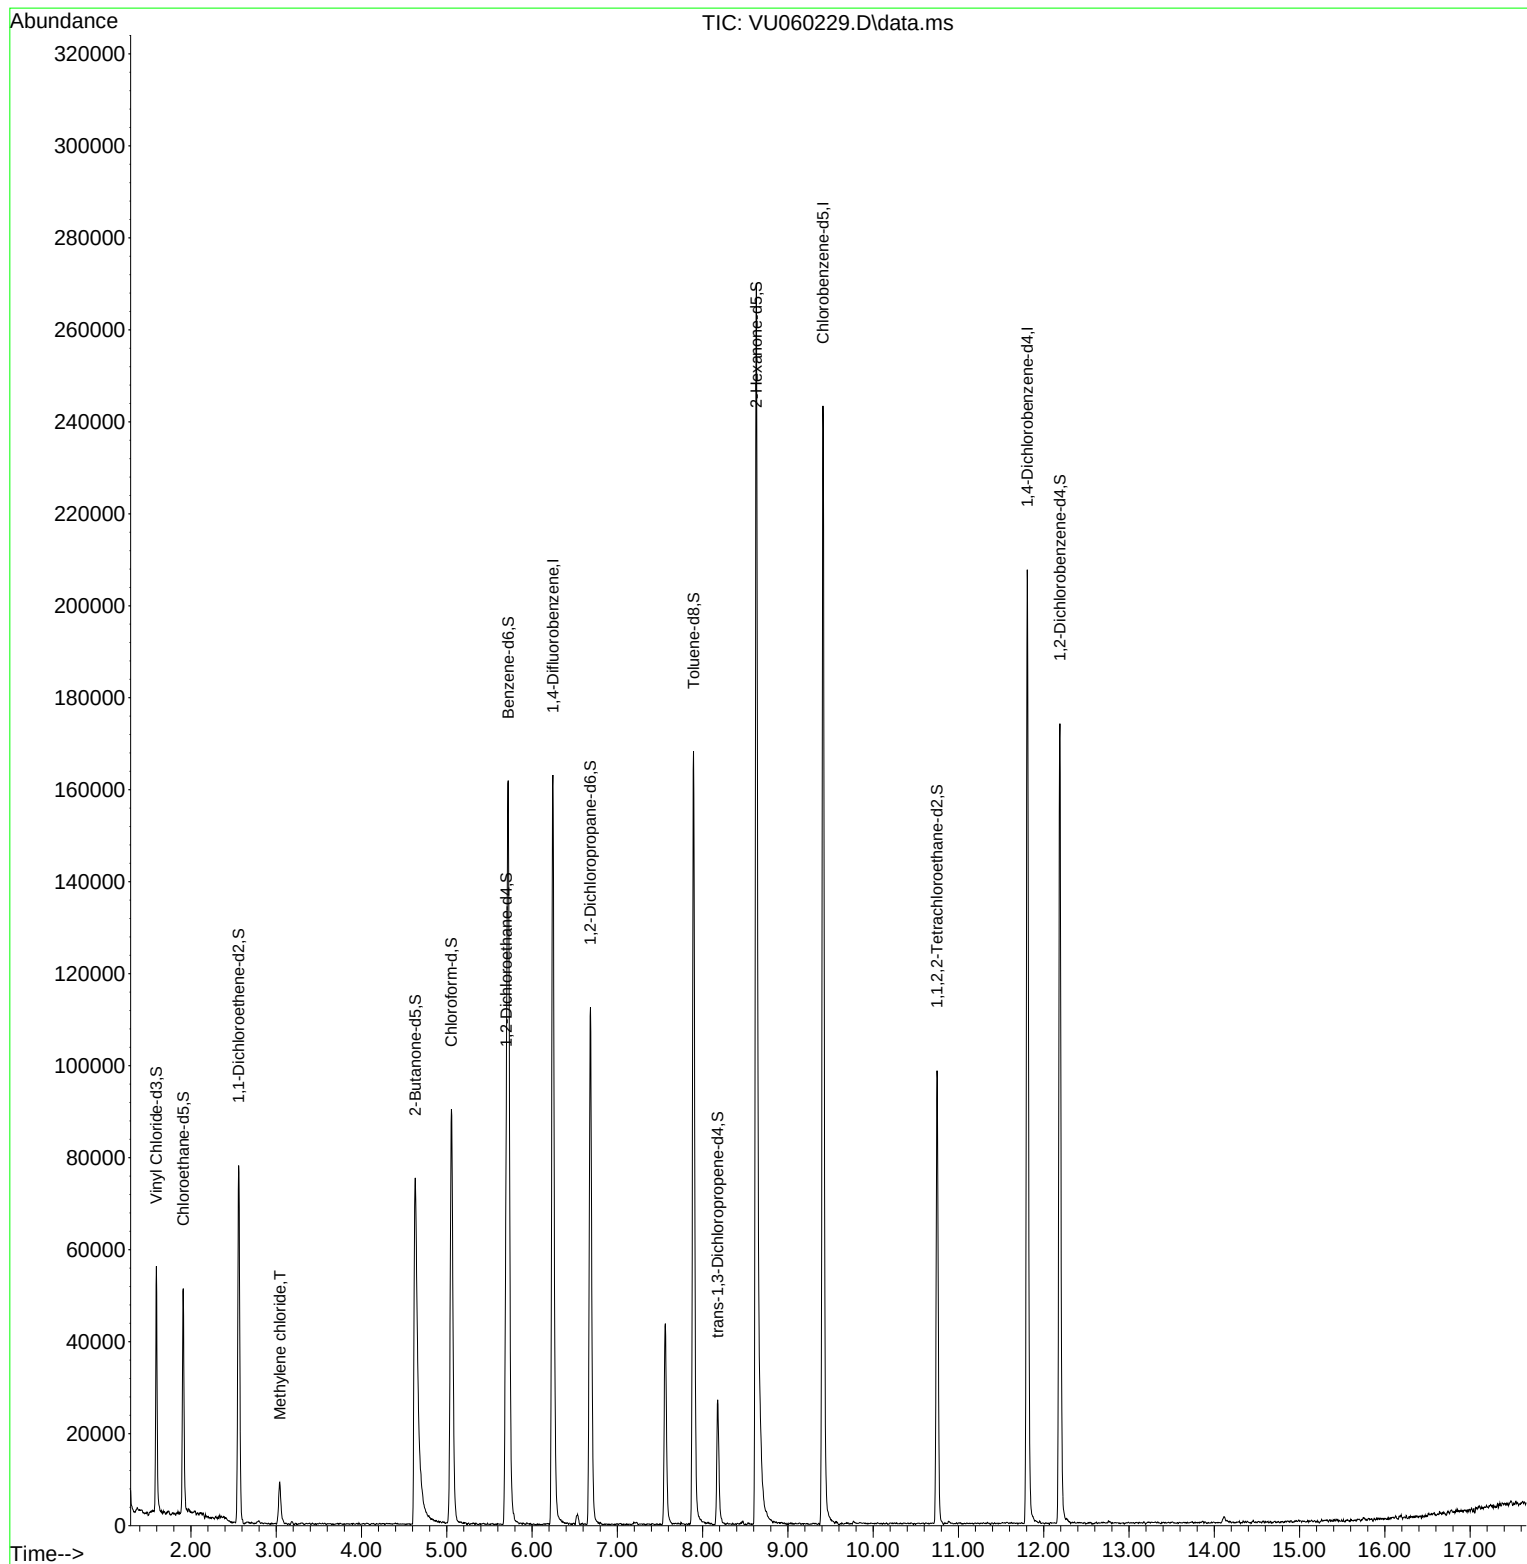

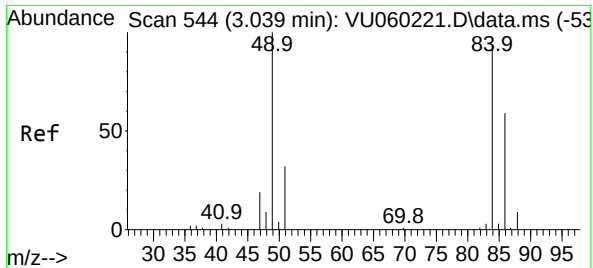

#16
Methylene chloride
Concen: 0.379 ug/L
RT: 3.042 min Scan# 54
Delta R.T. 0.003 min
Lab File: VU060229.D
Acq: 26 Jul 2024 17:24

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

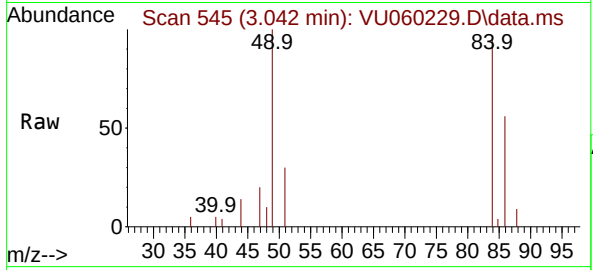

Tgt Ion:	84	Resp:	4898
Ion	Ratio	Lower	Upper
84	100		
86	58.7	44.4	82.5
49	105.7	72.0	133.6

