

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072624\
 Data File : VU060231.D
 Acq On : 26 Jul 2024 18:12
 Operator : MD/SY
 Sample : P3359-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1G98

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 07/30/2024
 Supervised By :Semsettin Yesilyurt 07/30/2024

Quant Time: Jul 26 23:17:53 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jul 26 23:14:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	134664	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	141884	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	59367	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	37513	4.004	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	80.000%	
7) Chloroethane-d5	1.911	69	37619	4.322	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	86.400%	
11) 1,1-Dichloroethene-d2	2.560	65	13854	3.787	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	75.800%	
20) 2-Butanone-d5	4.624	46	136945	62.517	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	125.040%	
24) Chloroform-d	5.055	84	85326	4.333	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	86.600%	
26) 1,2-Dichloroethane-d4	5.698	65	43298	4.722	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	94.400%	
32) Benzene-d6	5.721	84	151998	3.998	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	80.000%	
36) 1,2-Dichloropropane-d6	6.685	67	57714	4.765	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	95.200%	
41) Toluene-d8	7.894	98	112094	3.264	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	65.200%#	
43) trans-1,3-Dichloroprop...	8.177	79	18112	4.392	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	87.800%	
46) 2-Hexanone-d5	8.627	63	95380	52.127	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	104.260%	
56) 1,1,2,2-Tetrachloroeth...	10.750	84	52011	4.824	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	96.400%	
66) 1,2-Dichlorobenzene-d4	12.190	152	49611	4.630	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	92.600%	
Target Compounds						
5) Vinyl chloride	1.602	62	29715	2.155	ug/L	97
13) Acetone	2.647	43	9516m	6.567	ug/L	
22) cis-1,2-Dichloroethene	4.660	96	44714	3.734	ug/L	96
42) Toluene	7.965	91	102506	2.055	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072624\
Data File : VU060231.D
Acq On : 26 Jul 2024 18:12
Operator : MD/SY
Sample : P3359-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
E1G98

Quant Time: Jul 26 23:17:53 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 26 23:14:26 2024
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

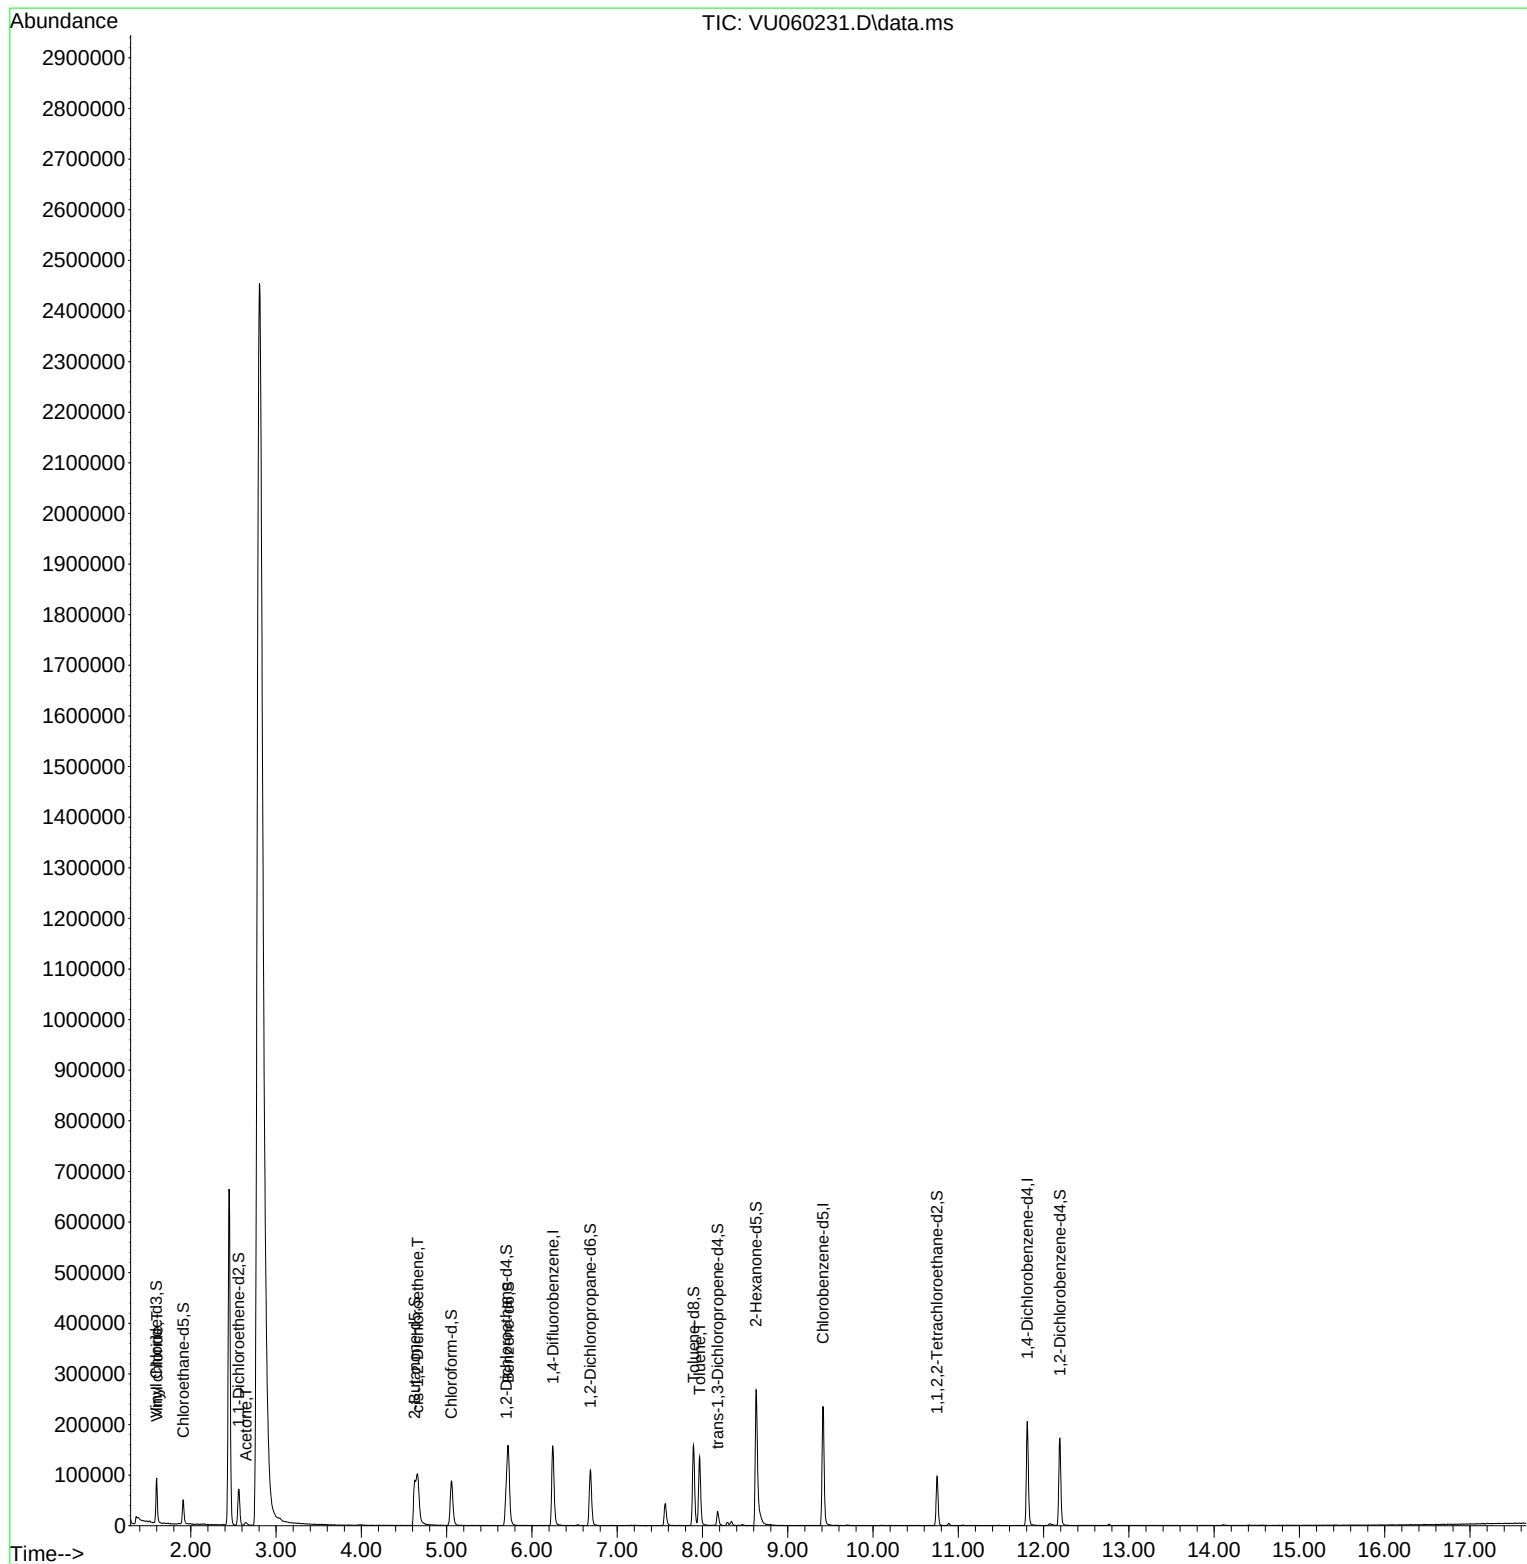

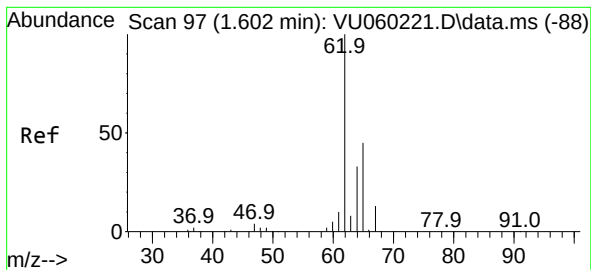

#5
 Vinyl chloride
 Concen: 2.155 ug/L
 RT: 1.602 min Scan# 97
 Delta R.T. 0.000 min
 Lab File: VU060231.D
 Acq: 26 Jul 2024 18:12




Instrument :
 MSVOA_U
 ClientSampleId :
 E1G98

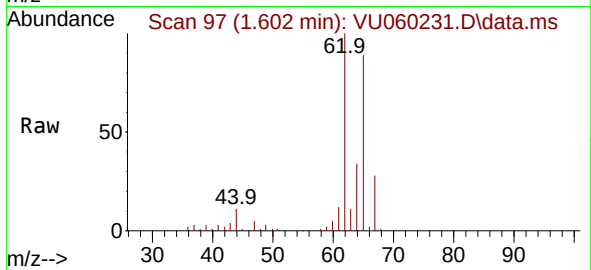

Tgt Ion: 62 Resp: 29715
 Ion Ratio Lower Upper
 62 100
 64 34.4 22.8 42.4




Manual Integrations
 APPROVED


Reviewed By :Mahesh Dadoda 07/30/2024
 Supervised By :Semsettin Yesilyurt 07/30/2024

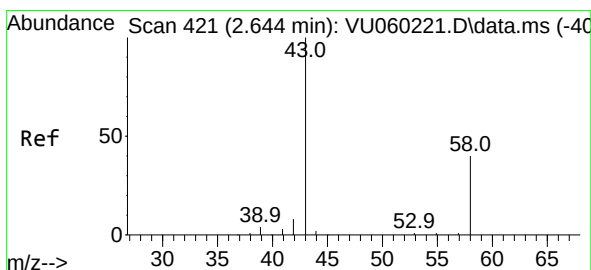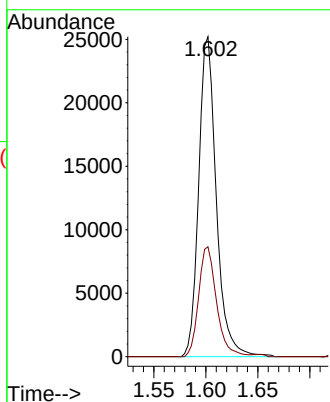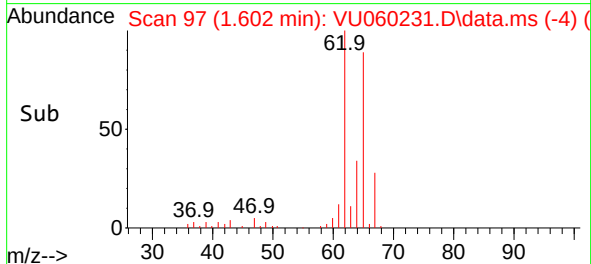

#13
 Acetone
 Concen: 6.567 ug/L m
 RT: 2.647 min Scan# 422
 Delta R.T. 0.003 min
 Lab File: VU060231.D
 Acq: 26 Jul 2024 18:12


Tgt Ion: 43 Resp: 9516
 Ion Ratio Lower Upper
 43 100
 58 34.9 0.0 82.2

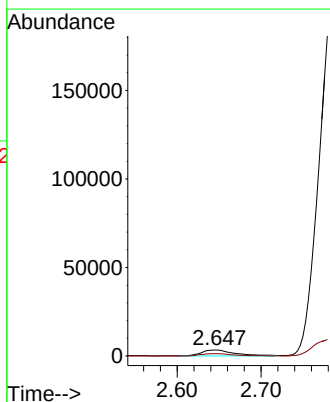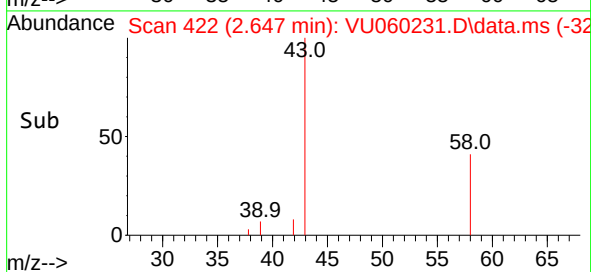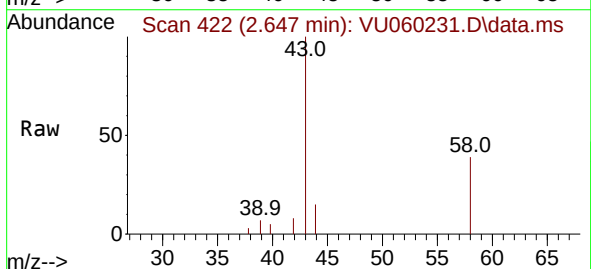

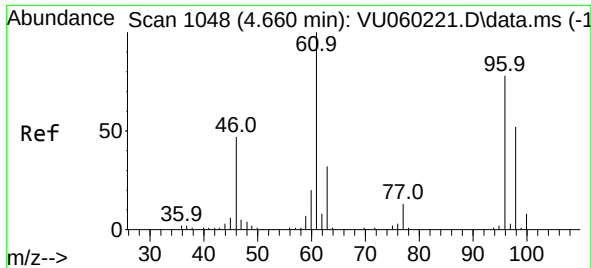

#22
cis-1,2-Dichloroethene
Concen: 3.734 ug/L
RT: 4.660 min Scan# 1048
Delta R.T. 0.000 min
Lab File: VU060231.D
Acq: 26 Jul 2024 18:12




Instrument :
MSVOA_U
ClientSampleId :
E1G98

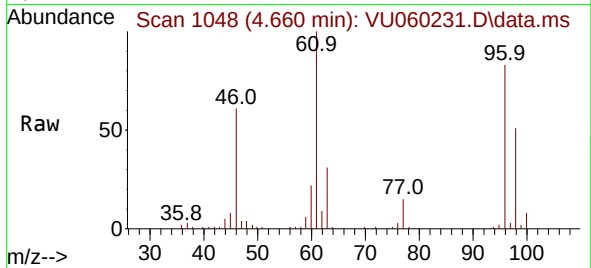


Tgt Ion: 96 Resp: 44714
Ion Ratio Lower Upper
96 100
61 120.4 80.2 148.9
98 62.0 44.7 83.1

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/30/2024
Supervised By :Semsettin Yesilyurt 07/30/2024

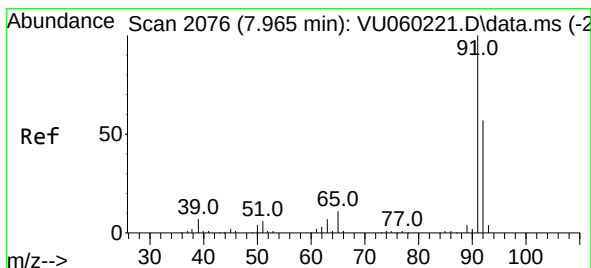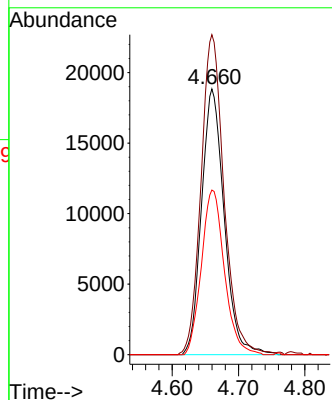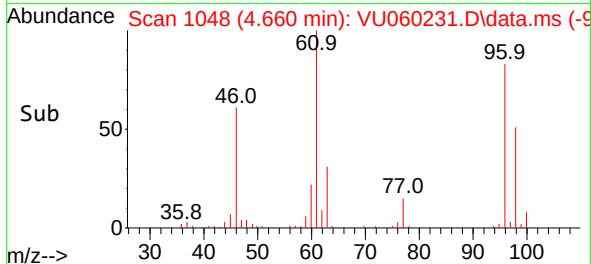

#42
Toluene
Concen: 2.055 ug/L
RT: 7.965 min Scan# 2076
Delta R.T. 0.000 min
Lab File: VU060231.D
Acq: 26 Jul 2024 18:12

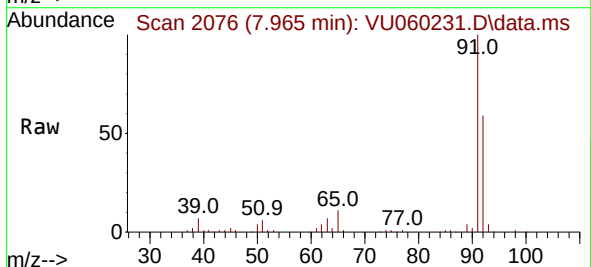

Tgt Ion: 91 Resp: 102506
Ion Ratio Lower Upper
91 100
92 59.5 39.8 73.8

