

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072624\
Data File : VU060233.D
Acq On : 26 Jul 2024 19:00
Operator : MD/SY
Sample : P3359-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GB9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU060233.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.447	348	360	382	rVB	197444	325807	3.96%	3.332%
2	2.640	407	420	449	rBV	55453	138170	1.68%	1.413%
3	2.814	449	474	532	rBV	1480189	8228616	100.00%	84.160%
4	6.245	1529	1541	1561	rBV	147679	291785	3.55%	2.984%
5	7.965	2065	2076	2092	rBV	51022	90552	1.10%	0.926%
6	9.412	2513	2526	2550	rBV	215125	369221	4.49%	3.776%
7	11.807	3258	3271	3297	rBV	191893	333223	4.05%	3.408%




Sum of corrected areas: 9777374

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072624\
Data File : VU060233.D
Acq On : 26 Jul 2024 19:00
Operator : MD/SY
Sample : P3359-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

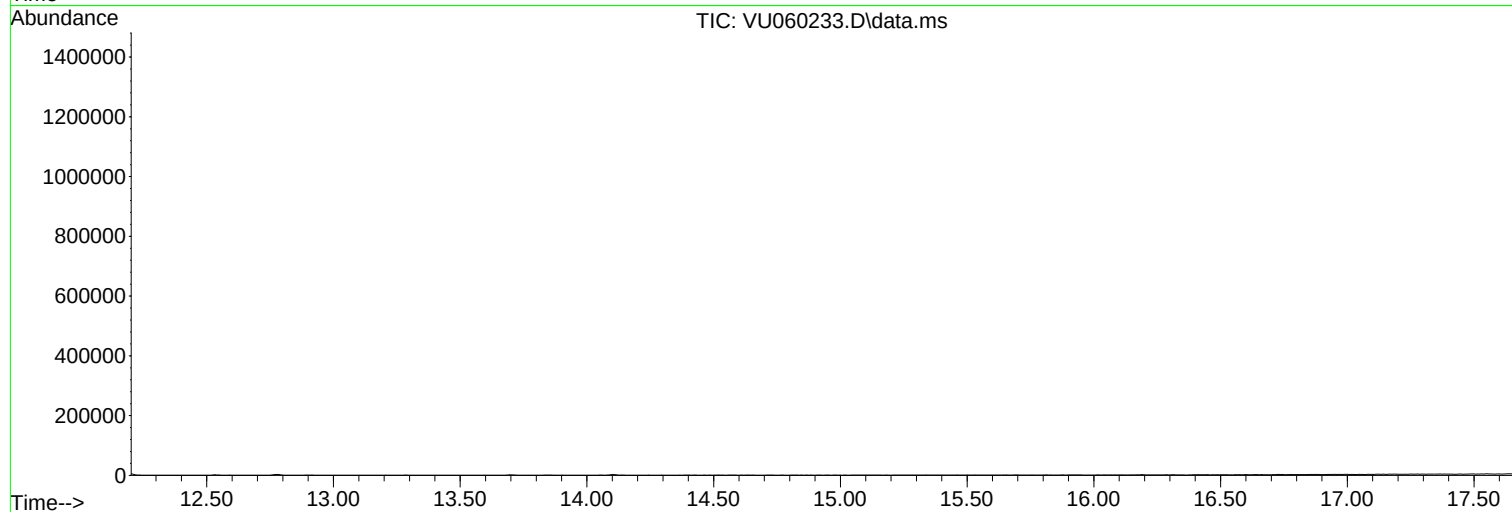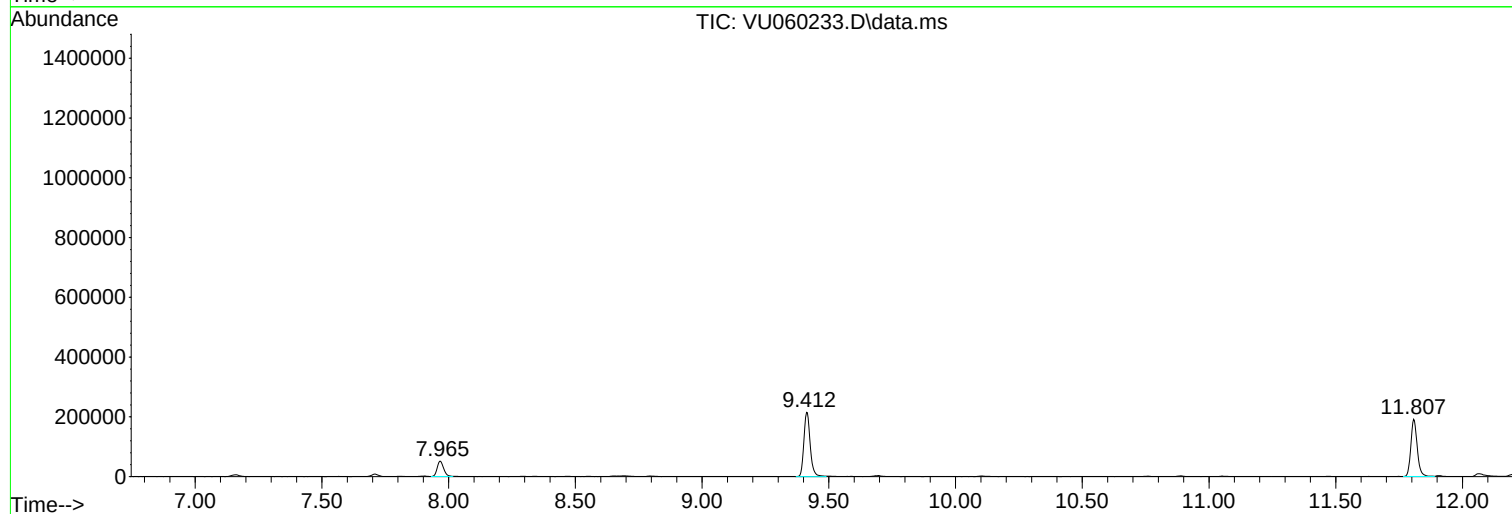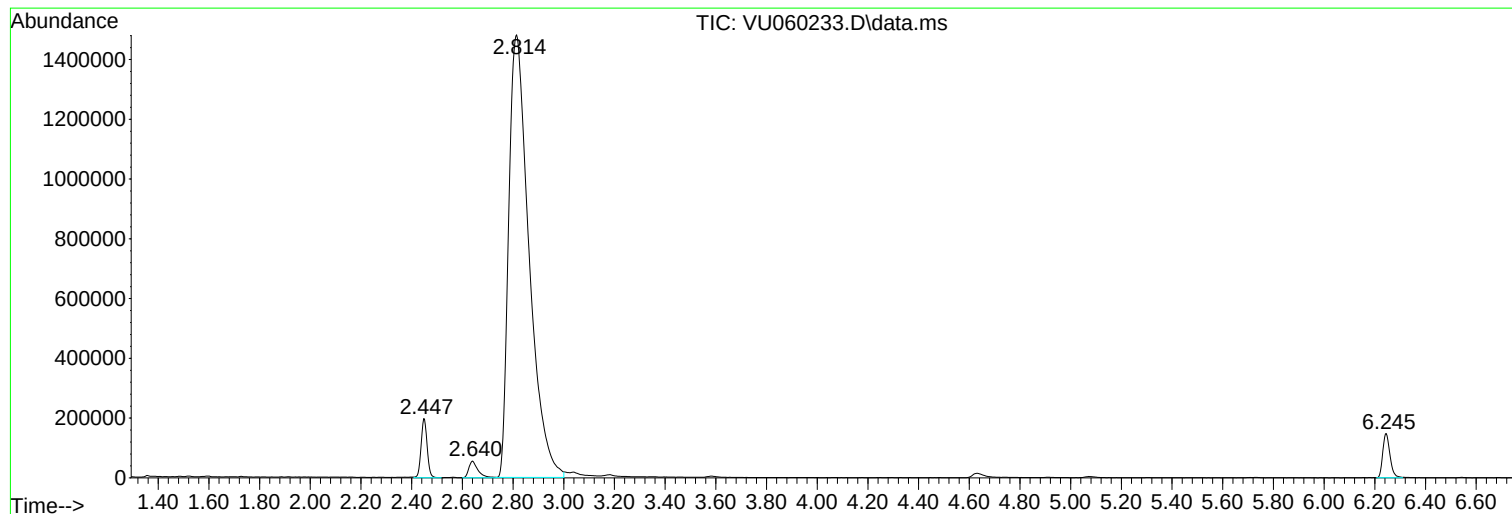

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072624\
Data File : VU060233.D
Acq On : 26 Jul 2024 19:00
Operator : MD/SY
Sample : P3359-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GB9










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.447	5.58 ug/L	325807	1,4-Difluorobenzene	6.245

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	91
2	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	72
3	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	58
4	Acetyl chloride			78	C2H3ClO	000075-36-5	9
5	2-Chloroethanol			80	C2H5ClO	000107-07-3	4

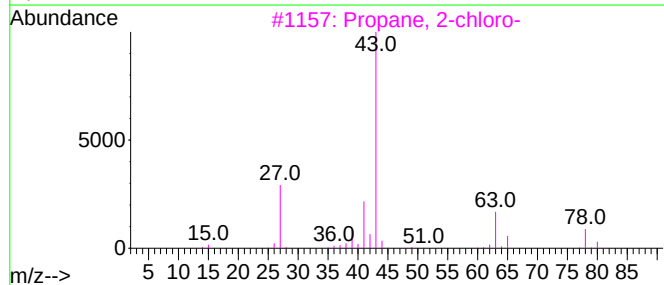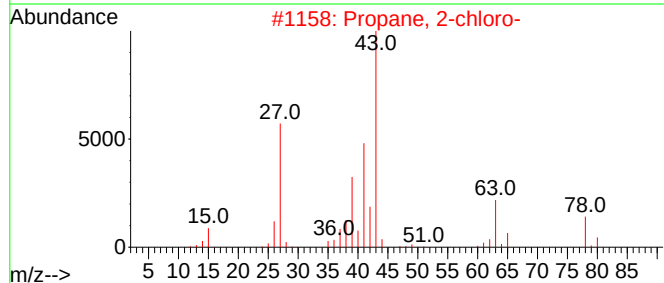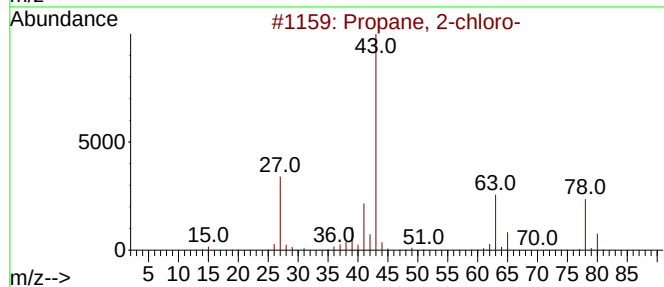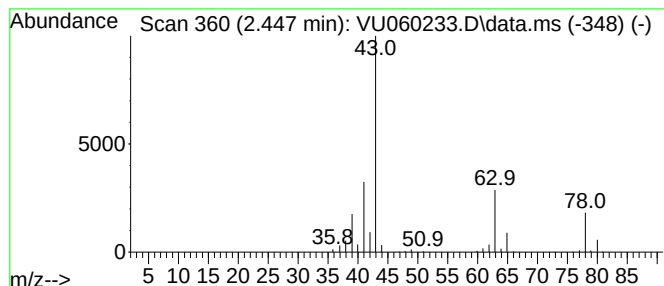

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072624\
Data File : VU060233.D
Acq On : 26 Jul 2024 19:00
Operator : MD/SY
Sample : P3359-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GB9










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.814	141.01 ug/L	8228620	1,4-Difluorobenzene	6.245

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Isopropyl Alcohol			60	C3H8O	000067-63-0	86
2	Isopropyl Alcohol			60	C3H8O	000067-63-0	78
3	Isopropyl Alcohol			60	C3H8O	000067-63-0	64
4	Isopropyl Alcohol			60	C3H8O	000067-63-0	56
5	Isopropyl Alcohol			60	C3H8O	000067-63-0	9

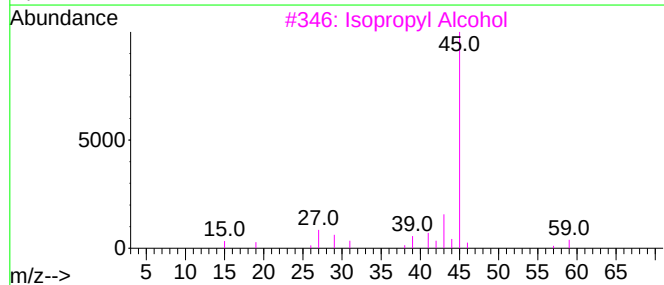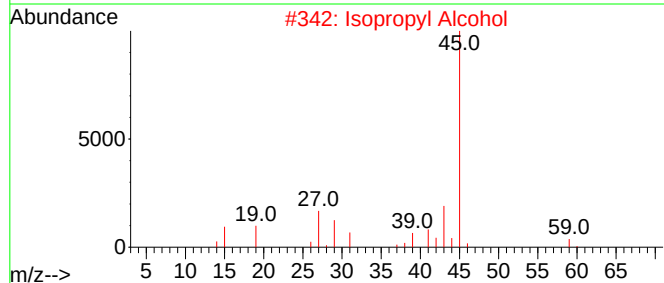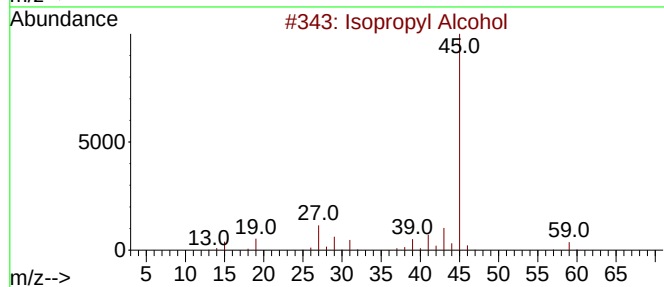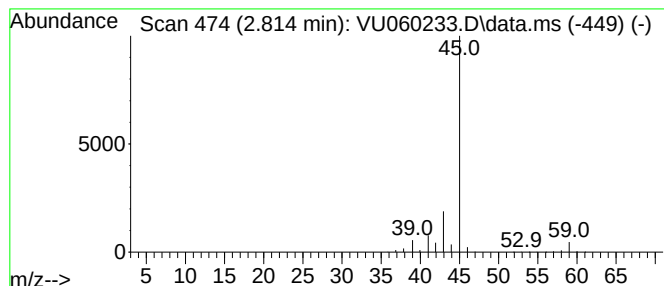

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072624\
Data File : VU060233.D
Acq On : 26 Jul 2024 19:00
Operator : MD/SY
Sample : P3359-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2-chloro-	2.447	5.6	ug/L	325807	1	6.245	291785	5.0
Isopropyl Alcohol	2.814	141.0	ug/L	8228620	1	6.245	291785	5.0