

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072624\
 Data File : VU060235.D
 Acq On : 26 Jul 2024 19:48
 Operator : MD/SY
 Sample : P3359-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GF0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU060235.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.448	348	360	381	rVB	663773	1085942	8.98%	6.355%
2	2.560	384	395	408	rBV	75419	124259	1.03%	0.727%
3	2.637	408	419	448	rBV	54688	134691	1.11%	0.788%
4	2.820	449	476	558	rBV2	1987587	12090056	100.00%	70.755%
5	4.627	1027	1038	1083	rBV	82303	246283	2.04%	1.441%
6	5.055	1157	1171	1195	rBV2	90813	205030	1.70%	1.200%
7	5.717	1358	1377	1410	rBV2	162225	438985	3.63%	2.569%
8	6.242	1528	1540	1562	rBV	183741	358903	2.97%	2.100%
9	6.685	1664	1678	1700	rBV	113470	223956	1.85%	1.311%
10	7.894	2042	2054	2071	rBV	162607	287569	2.38%	1.683%
11	8.631	2268	2283	2321	rBV2	270595	552997	4.57%	3.236%
12	9.412	2513	2526	2544	rBV	280033	471055	3.90%	2.757%
13	10.749	2930	2942	2963	rBV	100433	161869	1.34%	0.947%
14	11.807	3258	3271	3291	rBV	242094	397843	3.29%	2.328%
15	12.190	3378	3390	3414	rVB	184107	307761	2.55%	1.801%




Sum of corrected areas: 17087199

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072624\
Data File : VU060235.D
Acq On : 26 Jul 2024 19:48
Operator : MD/SY
Sample : P3359-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

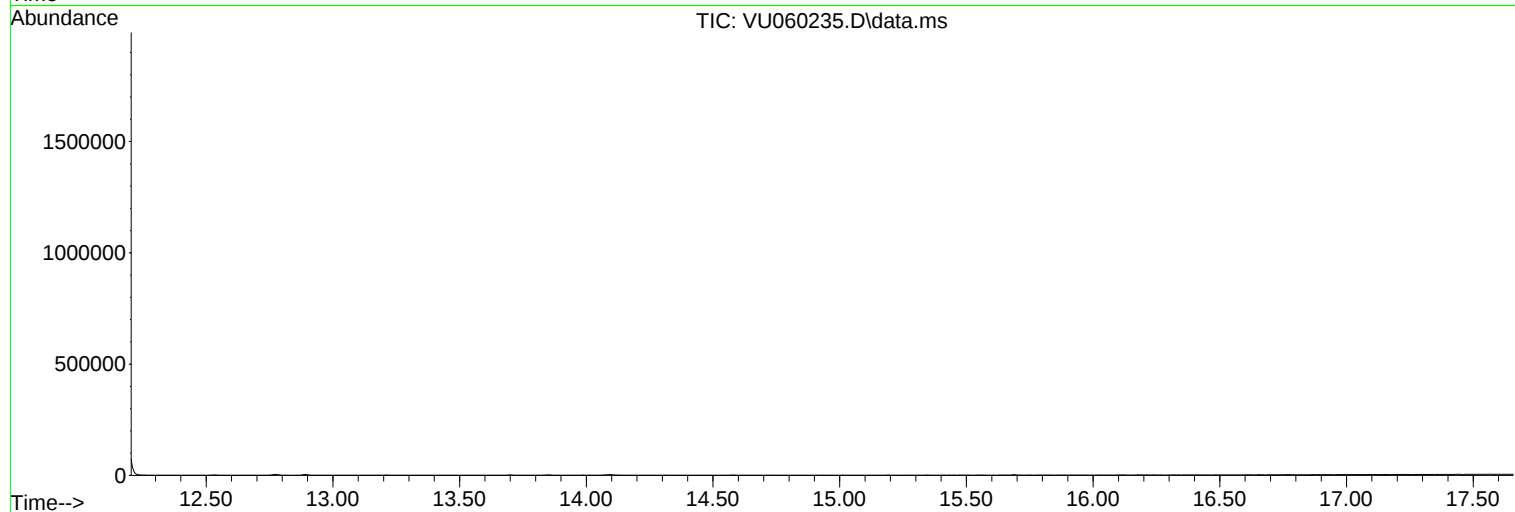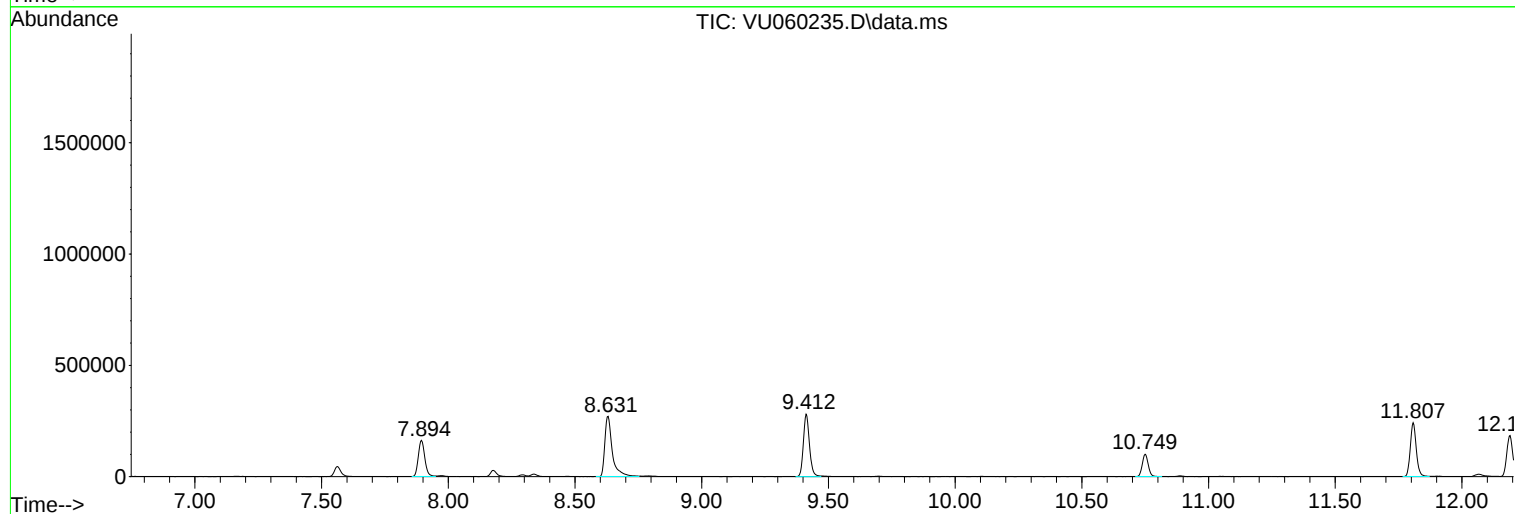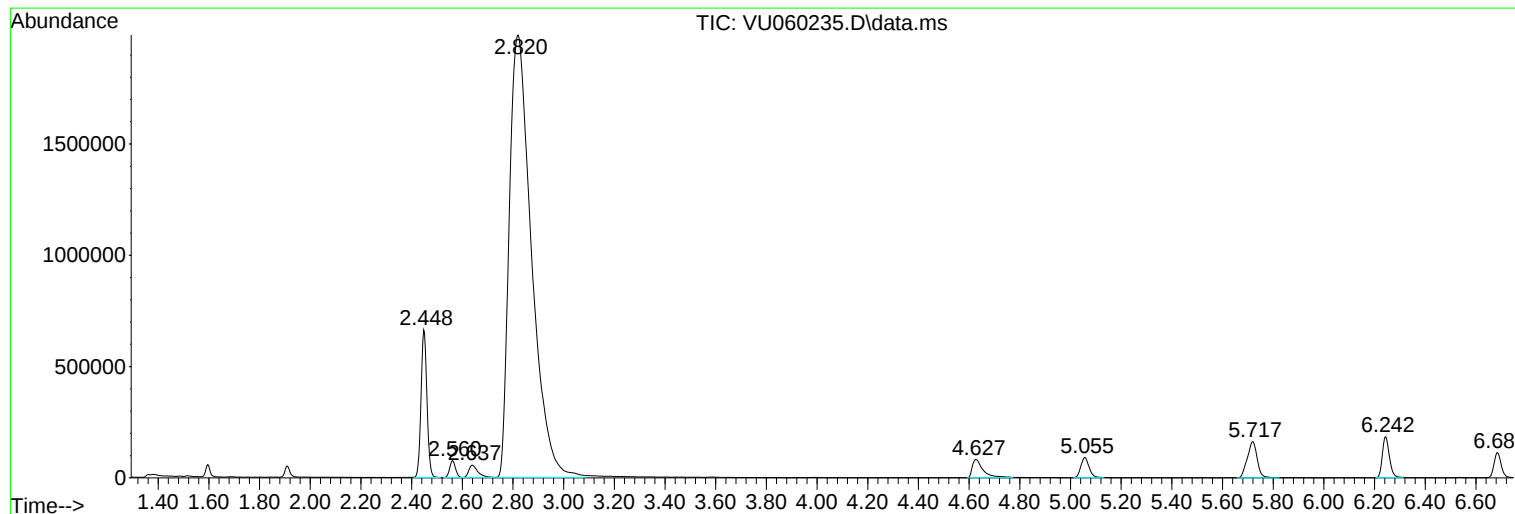

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072624\
Data File : VU060235.D
Acq On : 26 Jul 2024 19:48
Operator : MD/SY
Sample : P3359-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GF0







Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.448	15.13 ug/L	1085940	1,4-Difluorobenzene	6.245

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	91
2	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	58
3	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	42
4	Acetyl chloride			78	C2H3ClO	000075-36-5	9
5	2-Chloroethanol			80	C2H5ClO	000107-07-3	4

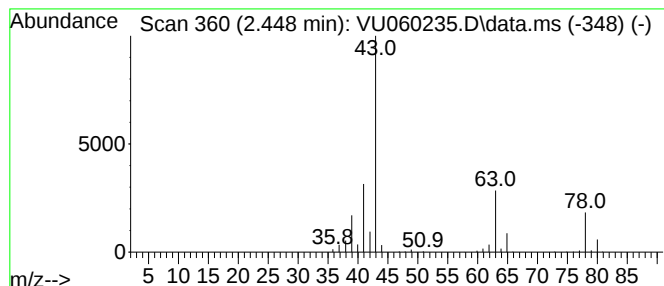

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072624\
Data File : VU060235.D
Acq On : 26 Jul 2024 19:48
Operator : MD/SY
Sample : P3359-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GF0










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.820	168.43 ug/L	12090100	1,4-Difluorobenzene	6.245

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	86
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
4			Hydrazine, ethyl-	60	C2H8N2	000624-80-6	9
5			Propanoic acid, 2-hydroxy-, meth...	104	C4H8O3	000547-64-8	9

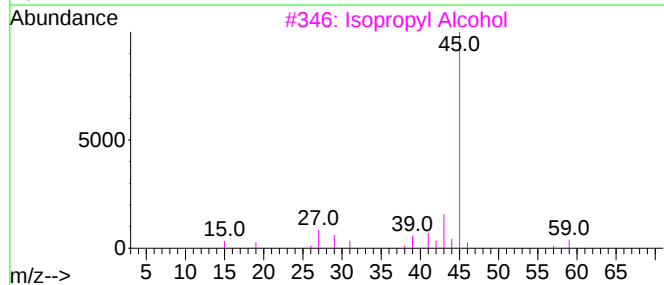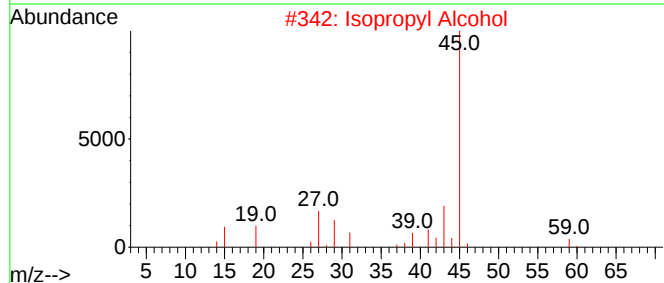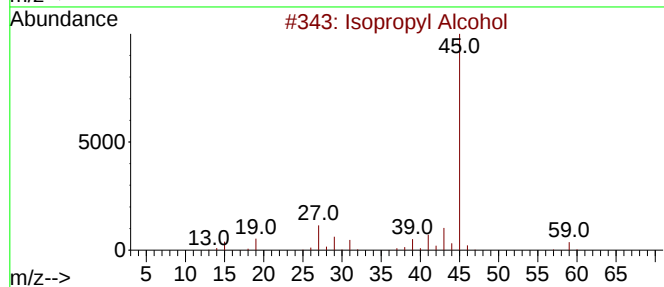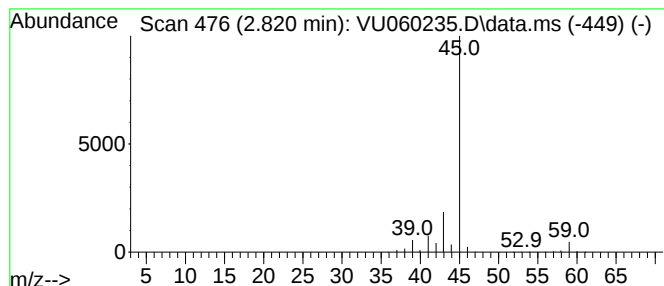

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072624\
Data File : VU060235.D
Acq On : 26 Jul 2024 19:48
Operator : MD/SY
Sample : P3359-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR071824WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2-chloro-	2.448	15.1	ug/L	1085940	1	6.245	358903	5.0
Isopropyl Alcohol	2.820	168.4	ug/L	12090100	1	6.245	358903	5.0