



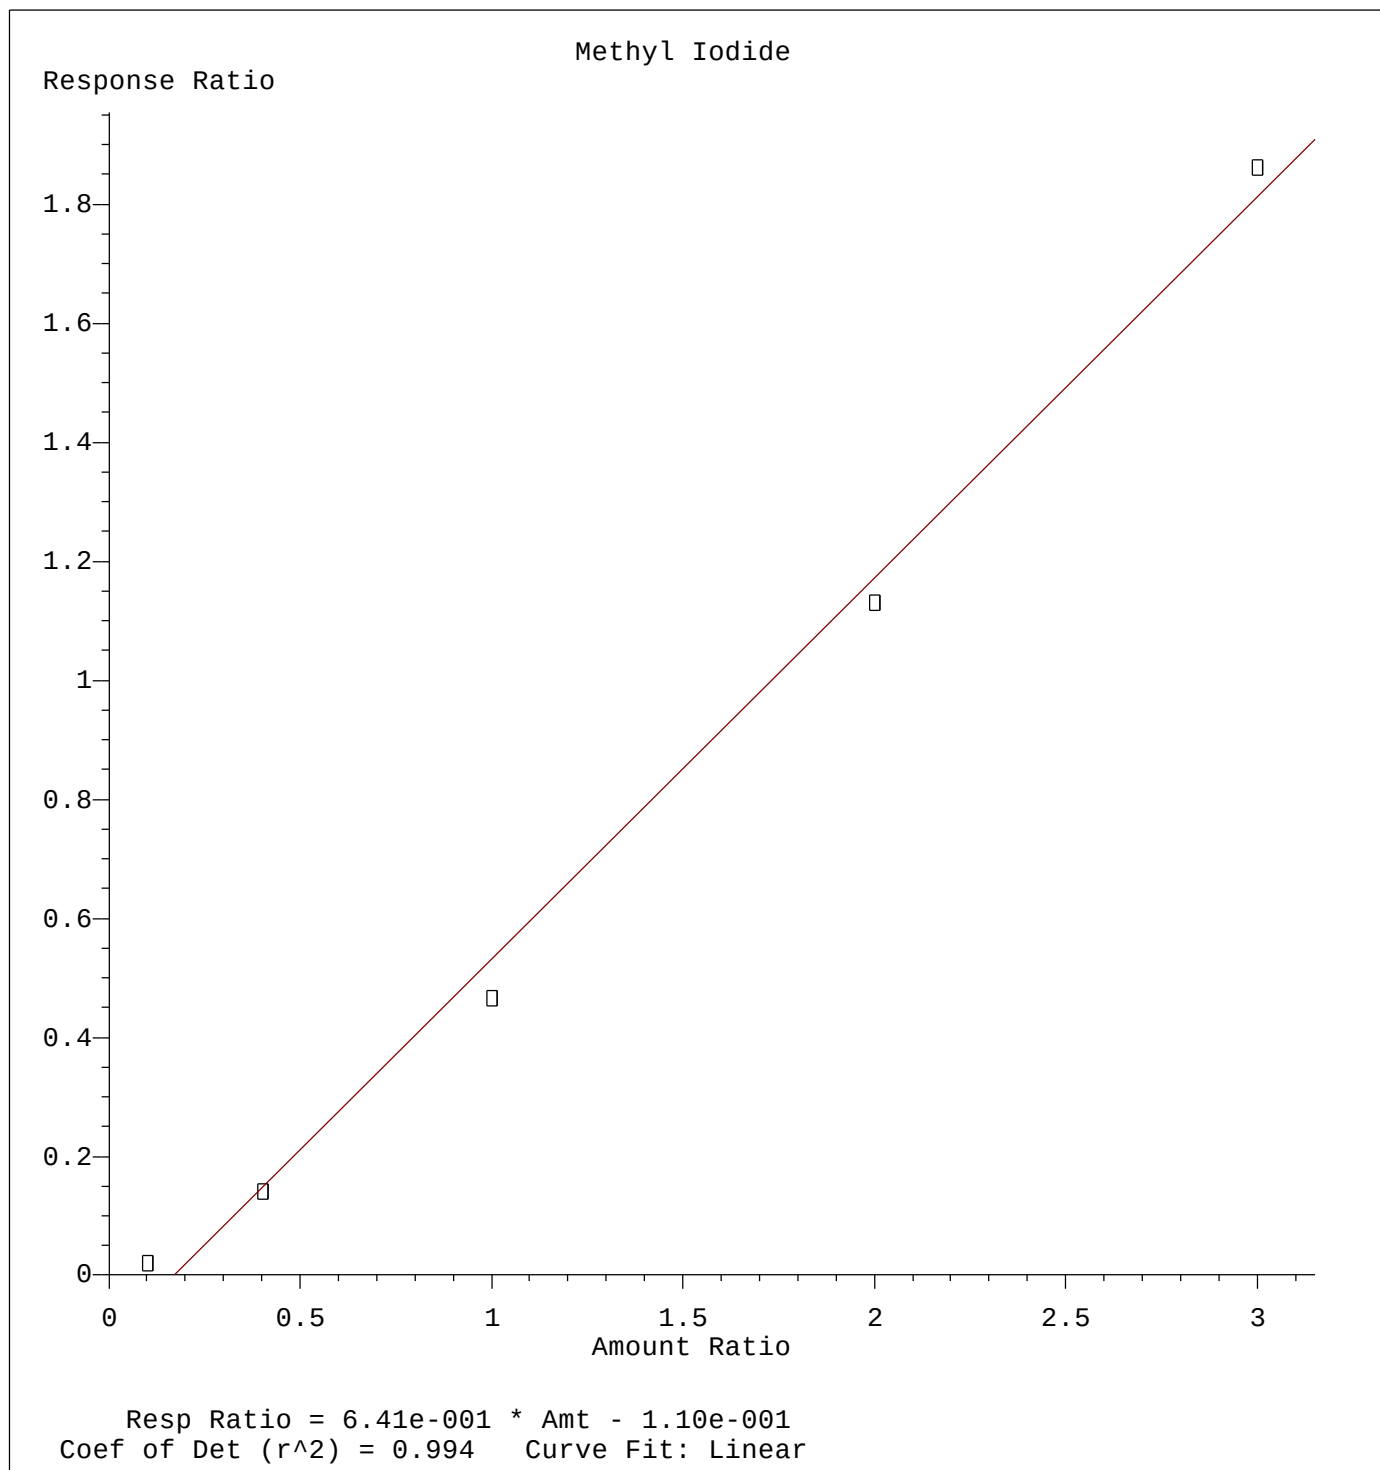

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\82U072718W.M  
Calibration Table Last Updated: Tue Jul 31 16:07:47 2018

# Naphthalene

Response Ratio

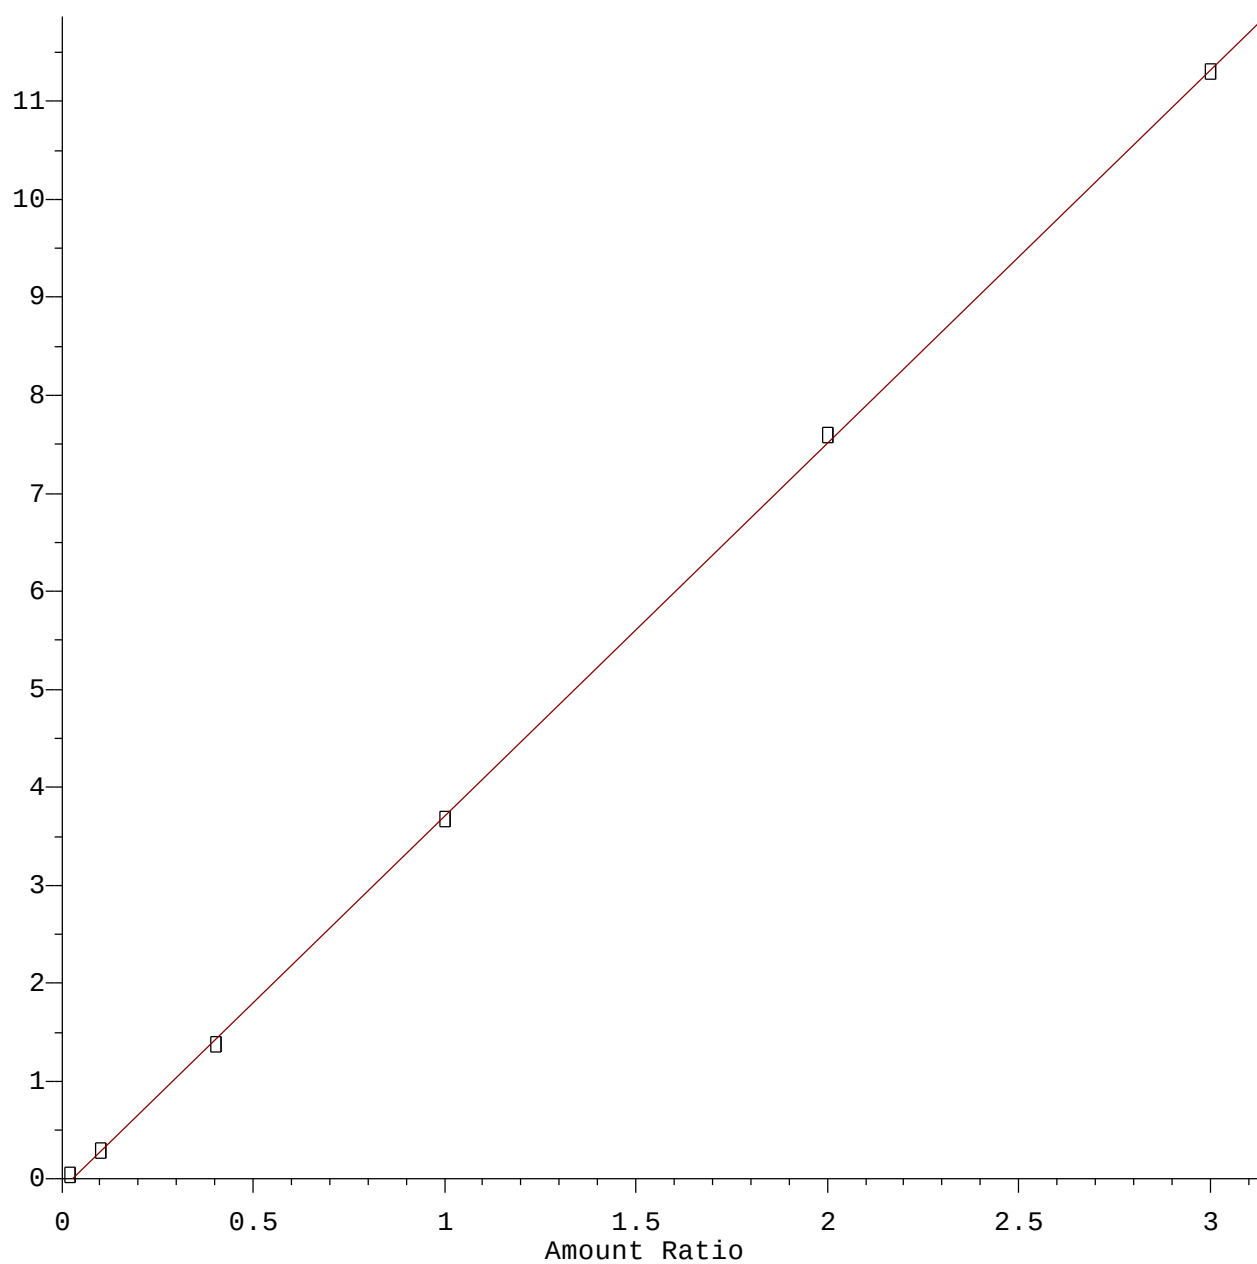


Resp Ratio = 3.81e+000 \* Amt - 9.53e-002  
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\82U072718W.M  
Calibration Table Last Updated: Tue Jul 31 16:07:47 2018


# 2-Chloroethyl Vinyl ether

Response Ratio

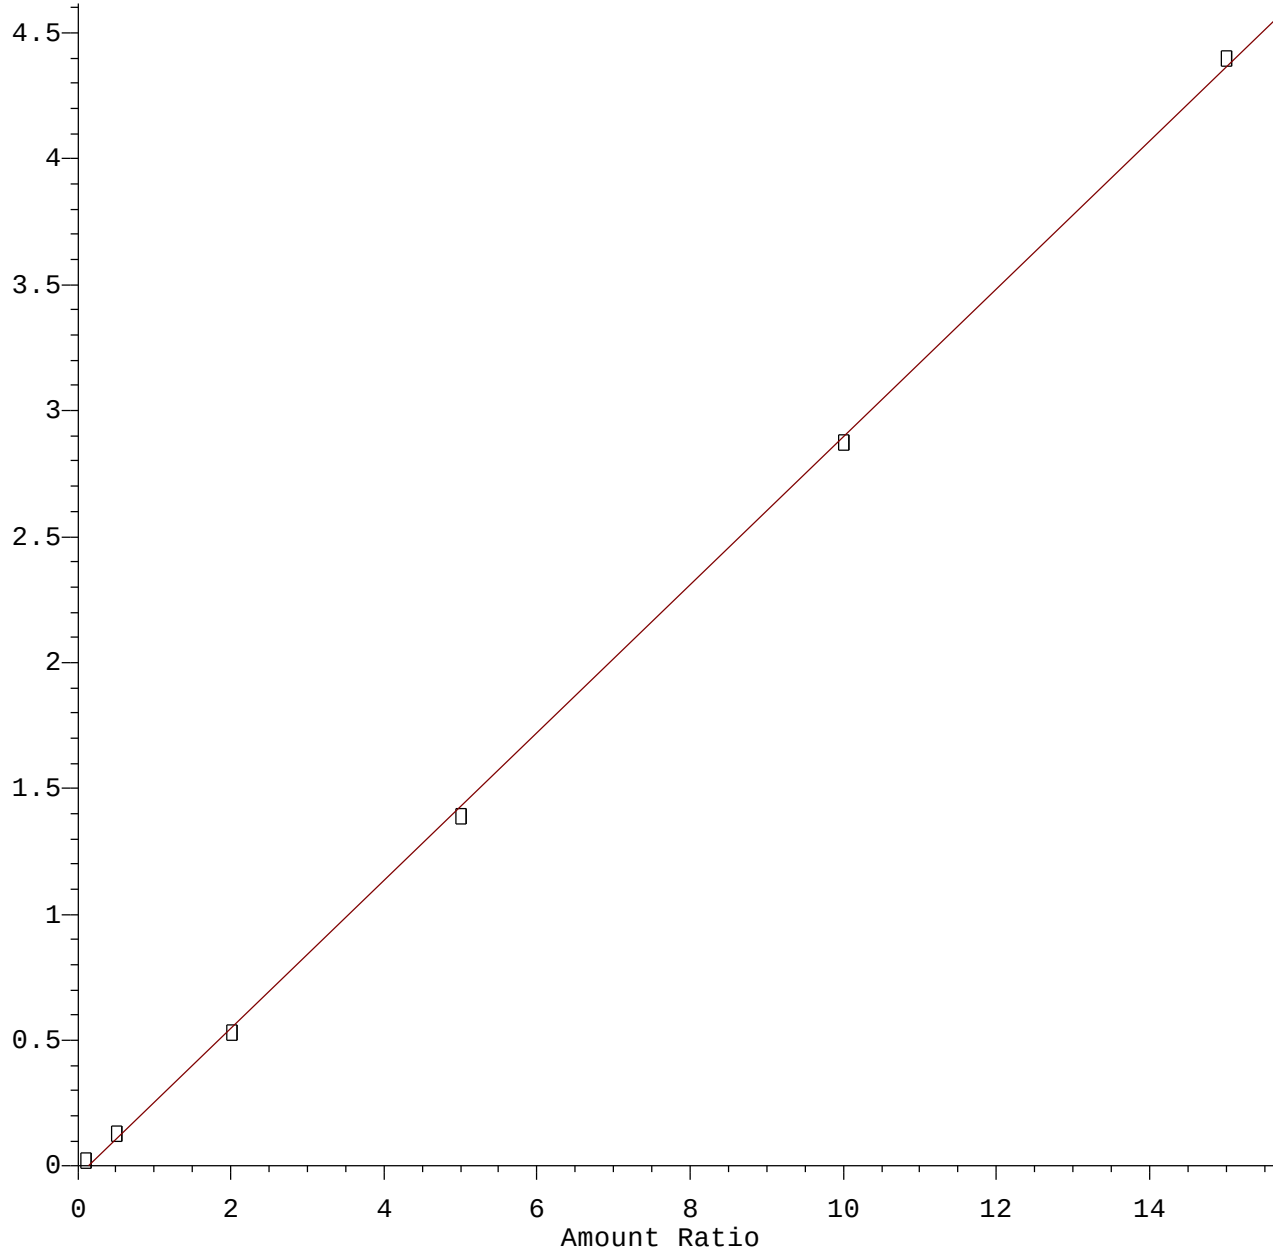

Resp Ratio =  $2.94 \times 10^{-1} \times \text{Amt} - 4.16 \times 10^{-2}$   
Coef of Det ( $r^2$ ) = 1.000 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\82U072718W.M  
Calibration Table Last Updated: Tue Jul 31 16:07:47 2018

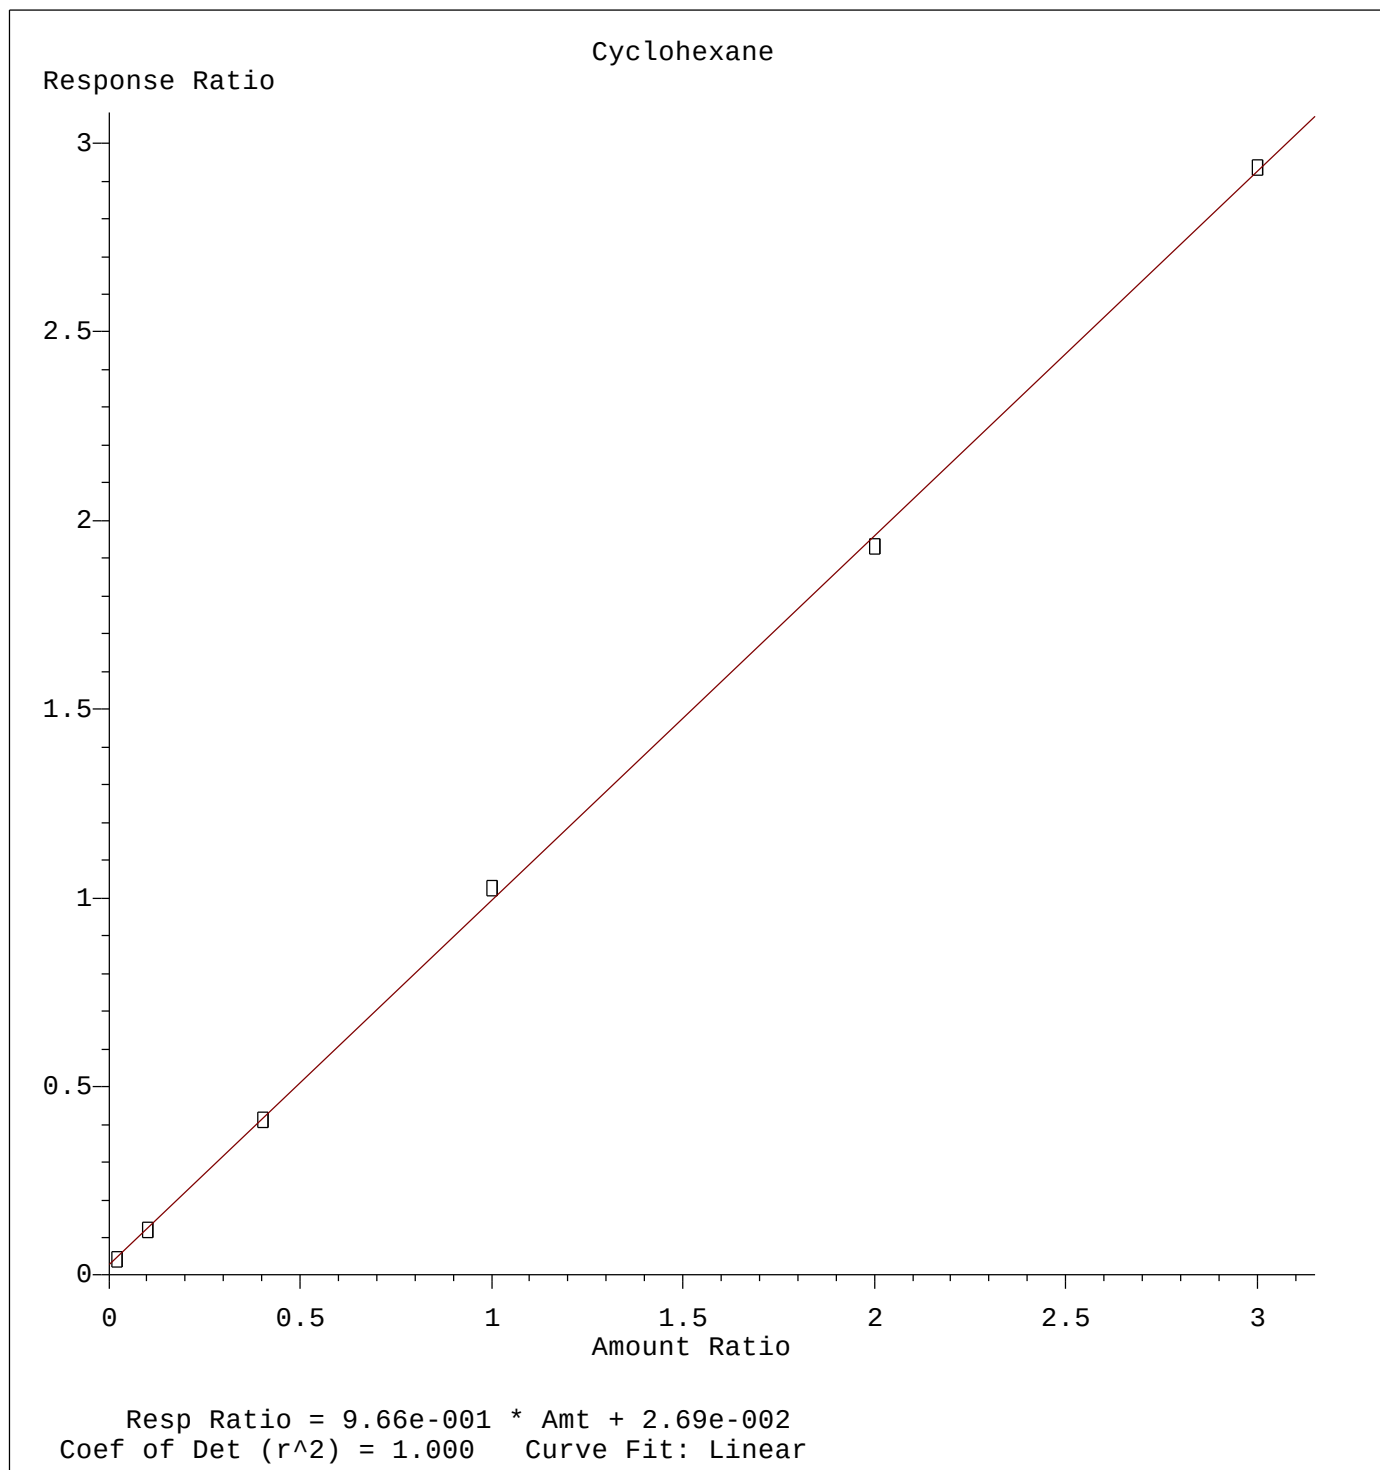

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\82U072718W.M  
Calibration Table Last Updated: Tue Jul 31 16:07:47 2018

# Acrolein

Response Ratio

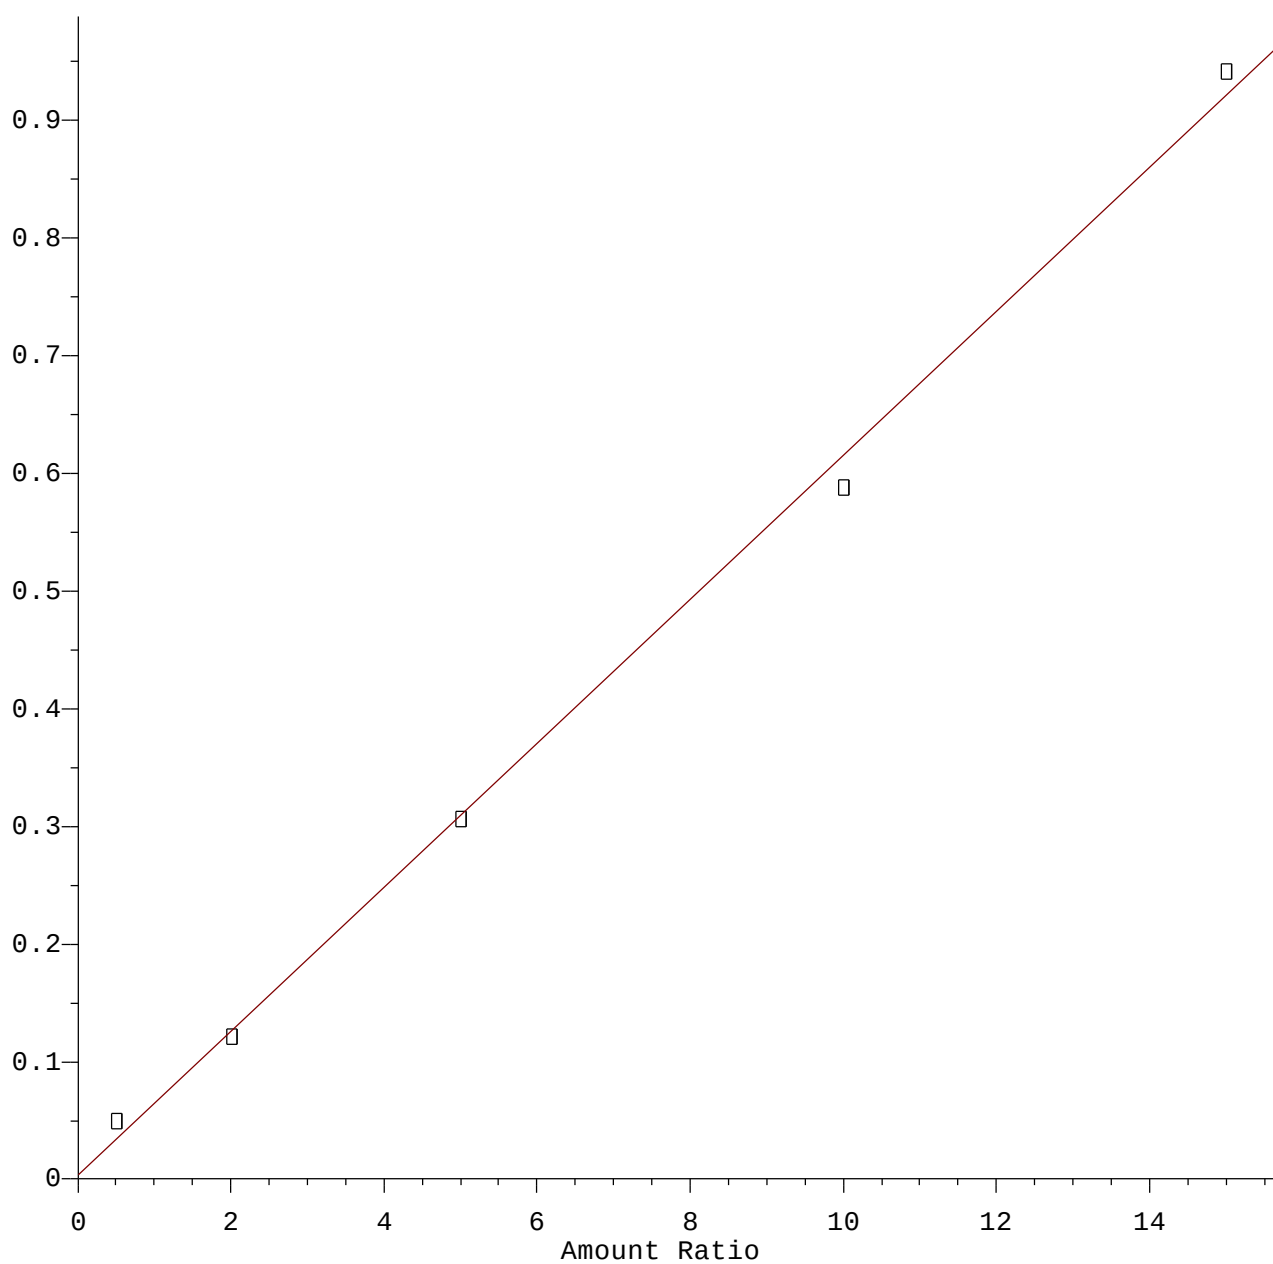

Resp Ratio =  $6.13 \times 10^{-2} \times \text{Amt} + 2.51 \times 10^{-3}$   
Coef of Det ( $r^2$ ) = 0.997    Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\82U072718W.M  
Calibration Table Last Updated: Tue Jul 31 16:07:47 2018