

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072718\
 Data File : VU025679.D
 Acq On : 27 Jul 2018 19:13
 Operator : MD/SY
 Sample : J4177-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TB01-072518

Quant Time: Jul 30 14:03:27 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U072718W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 27 13:11:52 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.99	168	175601	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.89	114	269258	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.09	117	262671	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.49	152	157959	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.32	65	133341	48.73	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.46%	
35) Dibromofluoromethane	4.89	113	110512	47.19	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.38%	
50) Toluene-d8	7.57	98	390317	47.63	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.26%	
62) 4-Bromofluorobenzene	10.31	95	149964	47.15	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.30%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU072718\
Data File : VU025679.D
Acq On : 27 Jul 2018 19:13
Operator : MD/SY
Sample : J4177-05
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TB01-072518

Quant Time: Jul 30 14:03:27 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U072718W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 27 13:11:52 2018
Response via : Initial Calibration

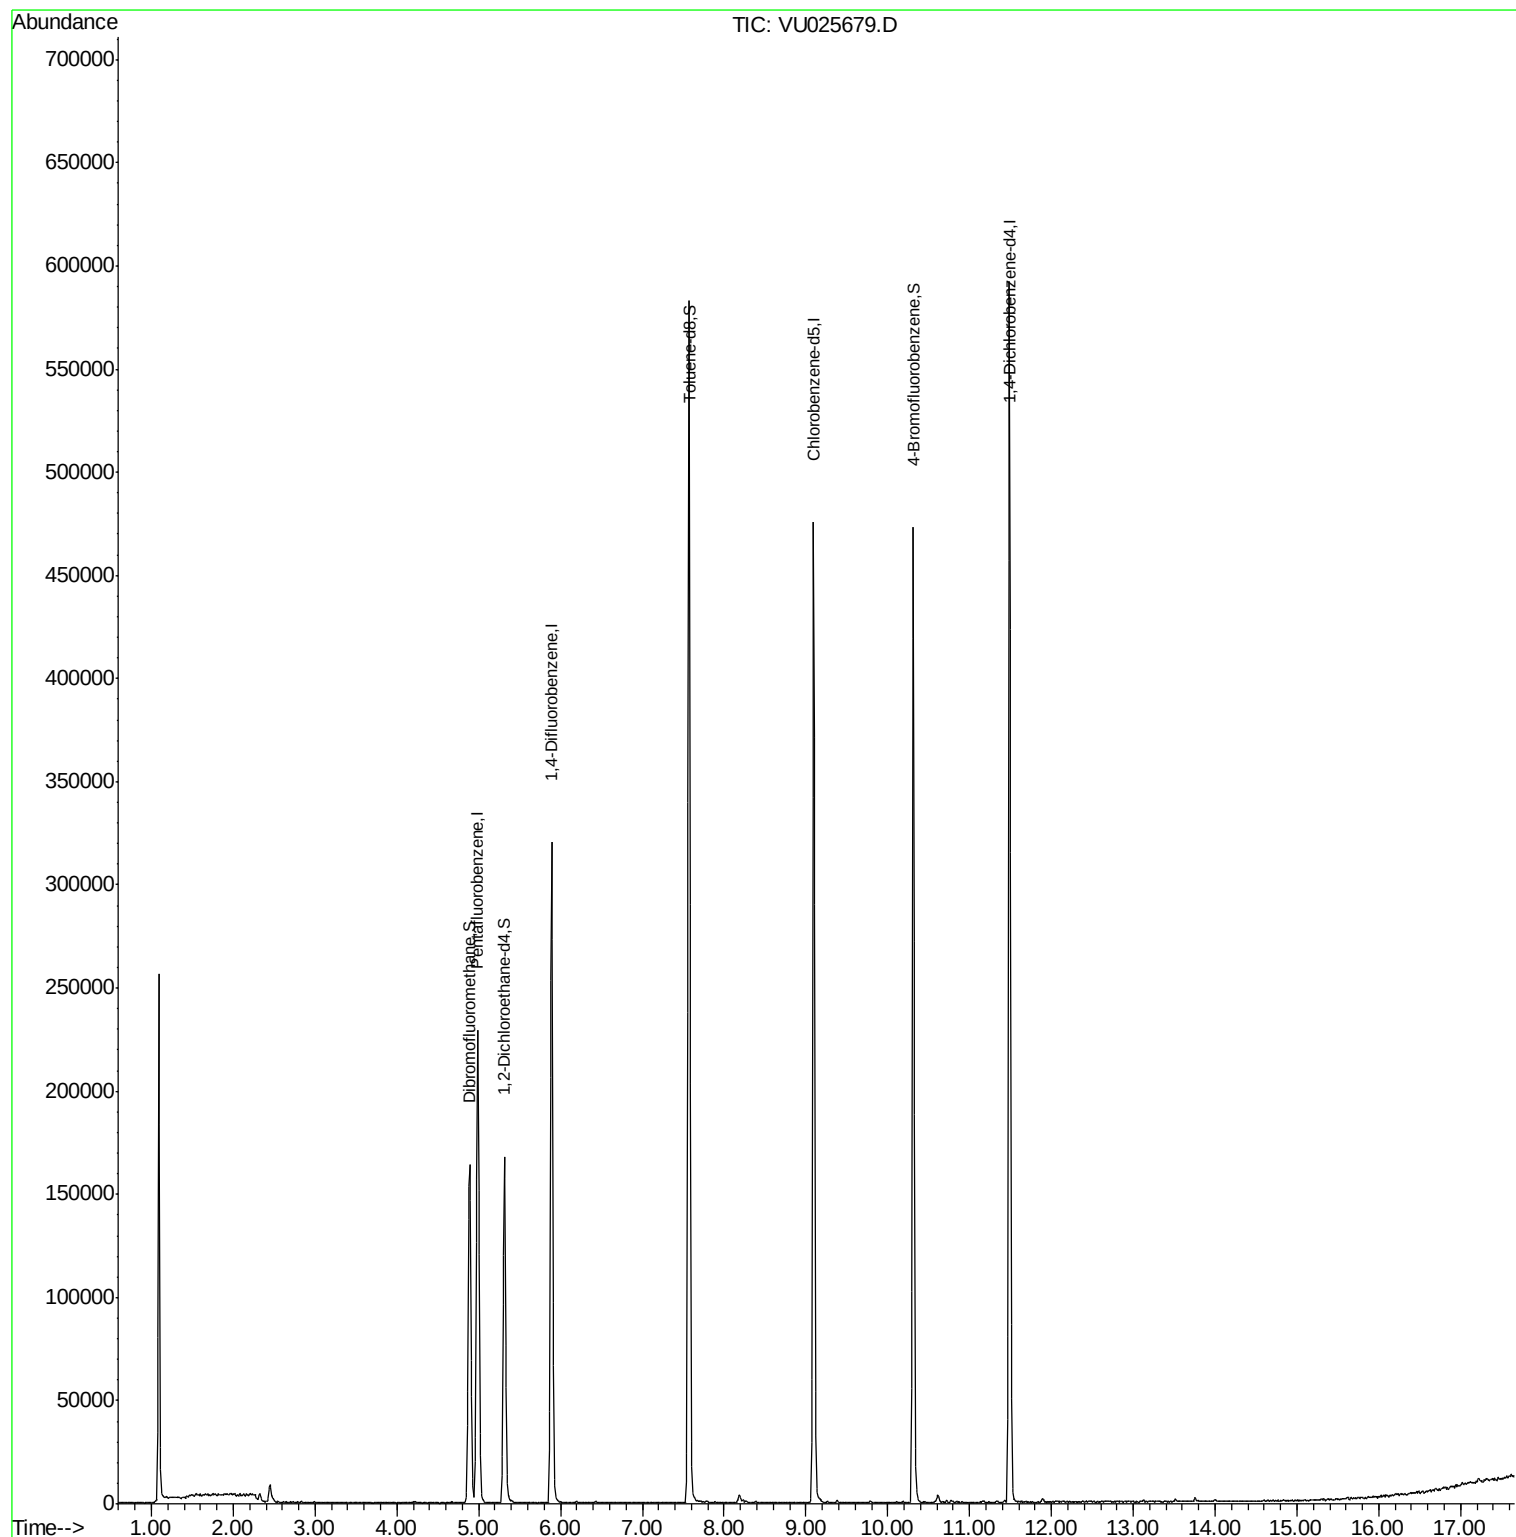

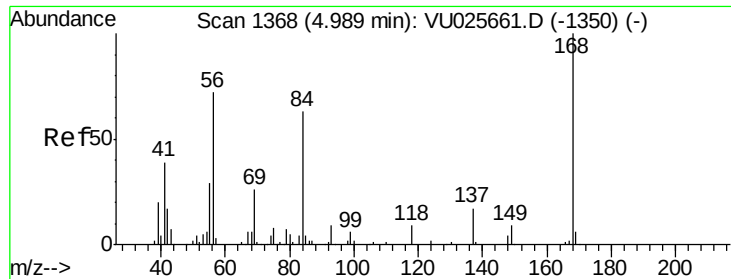

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 4.99 min Scan# 1368

Delta R.T. 0.00 min

Lab File: VU025679.D

Acq: 27 Jul 2018 19:13

Instrument :

MSVOA_U

ClientSampleId :


TB01-072518

Tot Ion:168 Resp: 175601

Ion Ratio Lower Upper




168 100

99 54.4 42.8 64.2

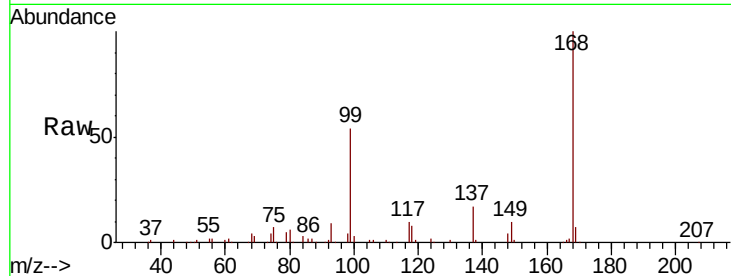

Abundance Ion 167.90 (167.60 to 168.60): VU025661.D (-1350) (-)

Ion 98.90 (98.60 to 99.60): VU025661.D (-1350) (-)

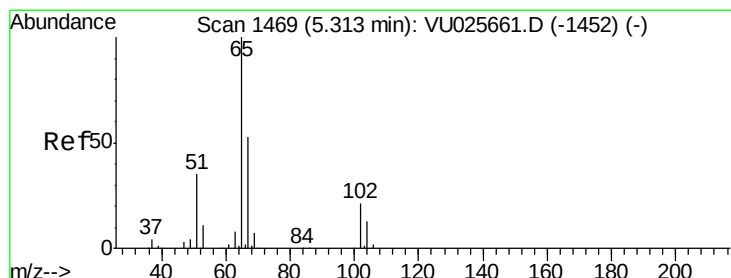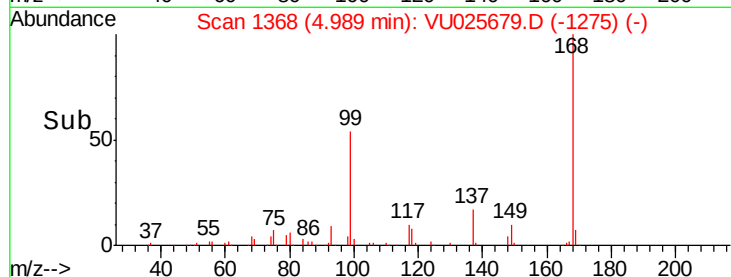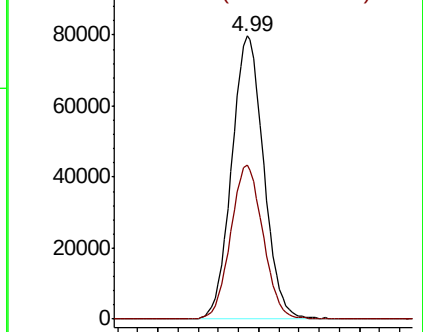

#33

1,2-Dichloroethane-d4

Concen: 48.73 ug/l

RT: 5.32 min Scan# 1470

Delta R.T. 0.00 min

Lab File: VU025679.D


Acq: 27 Jul 2018 19:13

Tgt Ion: 65 Resp: 133341

Ion Ratio Lower Upper



65 100


67 52.1 0.0 103.6

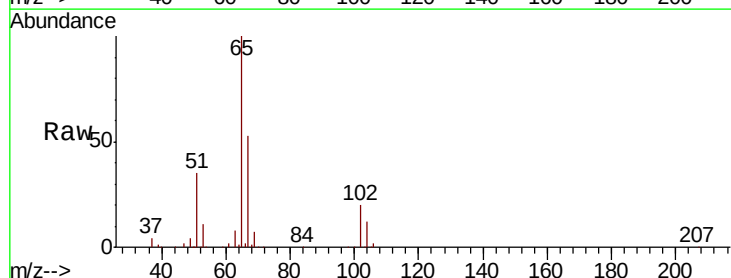

Abundance Ion 64.90 (64.60 to 65.60): VU025661.D (-1452) (-)

Ion 66.90 (66.60 to 67.60): VU025661.D (-1452) (-)

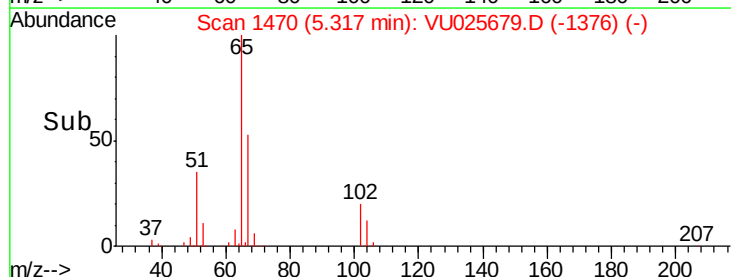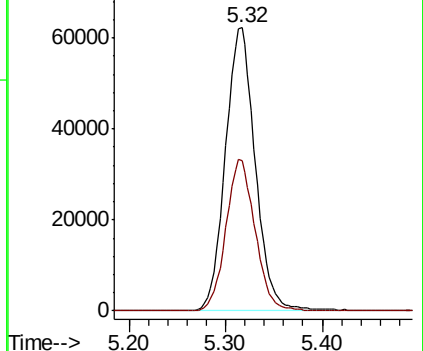

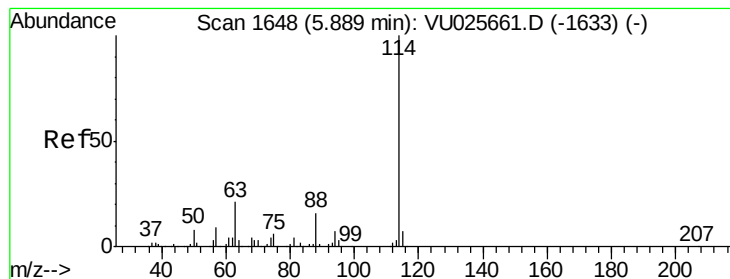

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 5.89 min Scan# 1649

Delta R.T. 0.00 min

Lab File: VU025679.D

Acq: 27 Jul 2018 19:13

Instrument :

MSVOA_U

ClientSampleId :

TB01-072518


Tot Ion:114 Resp: 269258

Ion Ratio Lower Upper

114 100

63 20.8 0.0 41.6




88 16.0 0.0 32.4

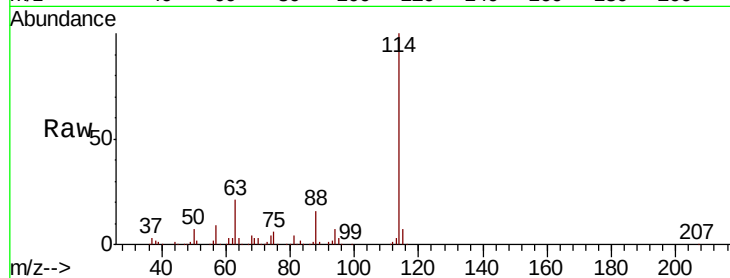

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VU0

Ion 87.90 (87.60 to 88.60): VU0

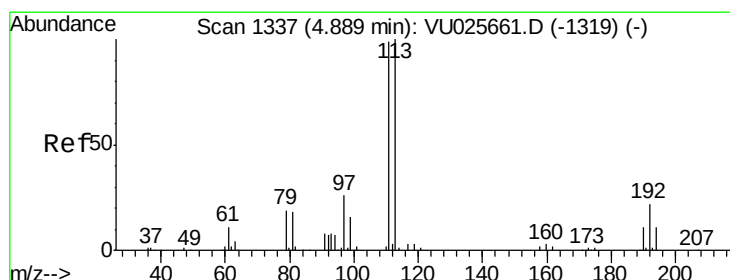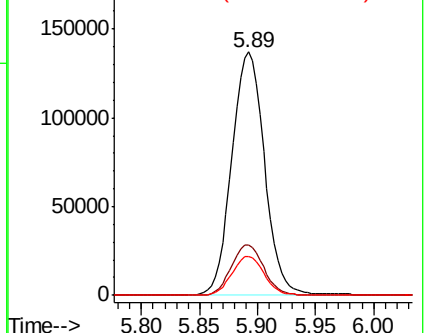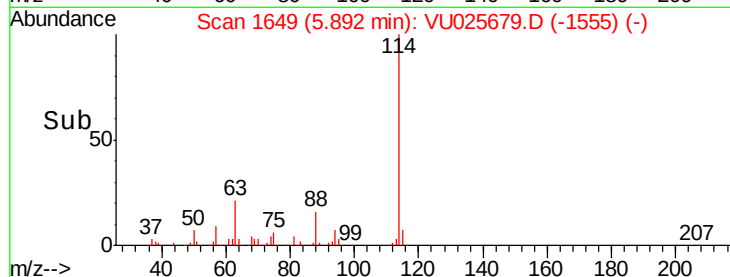

#35

Dibromofluoromethane

Concen: 47.19 ug/l

RT: 4.89 min Scan# 1337

Delta R.T. 0.00 min

Lab File: VU025679.D

Acq: 27 Jul 2018 19:13


Tgt Ion:113 Resp: 110512

Ion Ratio Lower Upper

113 100

111 102.7 81.7 122.5



192 21.1 17.1 25.7

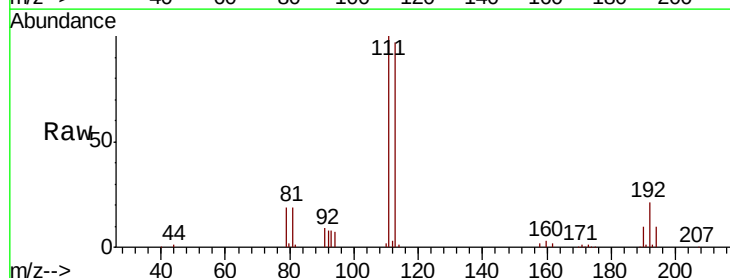


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



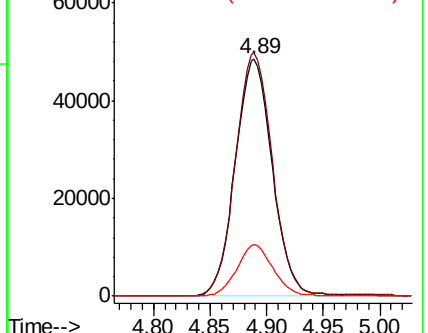
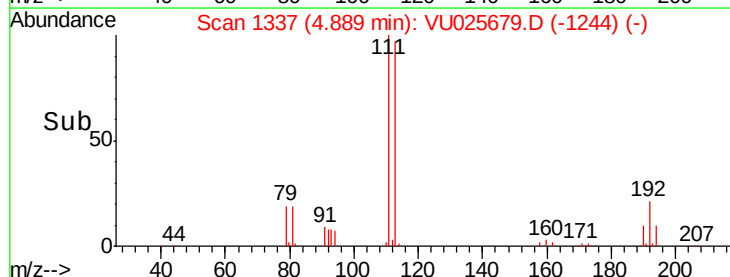


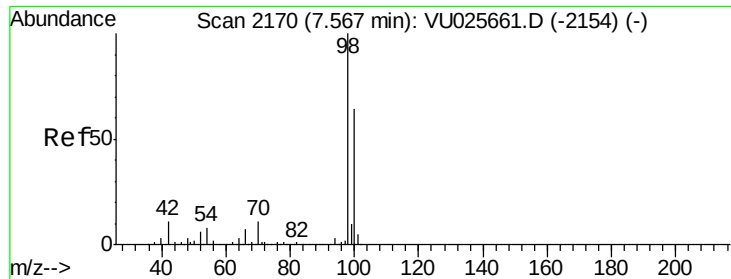

#50
Toluene-d8
Concen: 47.63 ug/l
RT: 7.57 min Scan# 2171
Delta R.T. 0.00 min
Lab File: VU025679.D
Acq: 27 Jul 2018 19:13




Instrument :
MSVOA_U
ClientSampleId :
TB01-072518


Tot Ion: 98 Resp: 390317
Ion Ratio Lower Upper
98 100
100 64.3 51.1 76.7

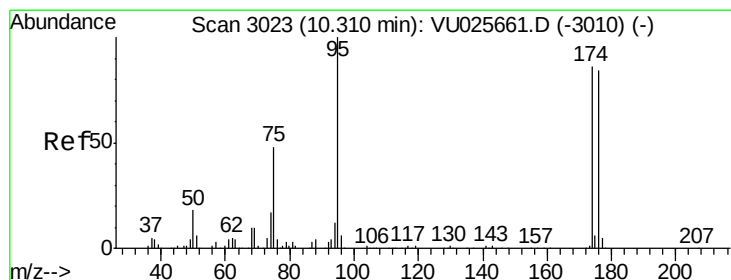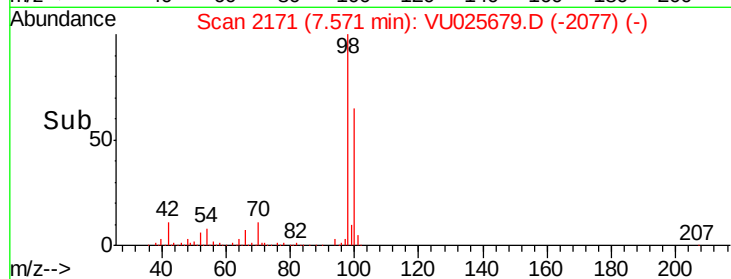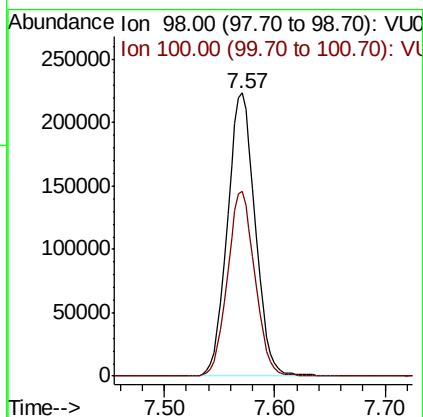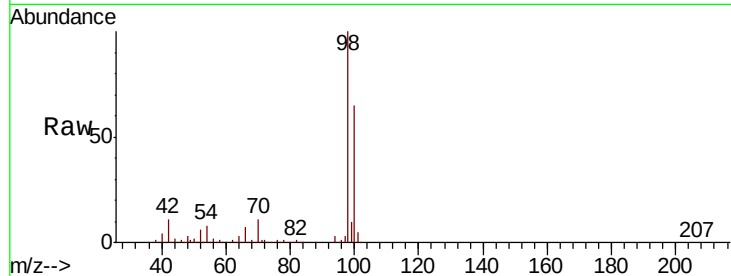

#62
4-Bromofluorobenzene
Concen: 47.15 ug/l
RT: 10.31 min Scan# 3023
Delta R.T. 0.00 min
Lab File: VU025679.D
Acq: 27 Jul 2018 19:13

Tgt Ion: 95 Resp: 149964
Ion Ratio Lower Upper
95 100
174 89.0 0.0 172.2
176 83.5 0.0 162.6


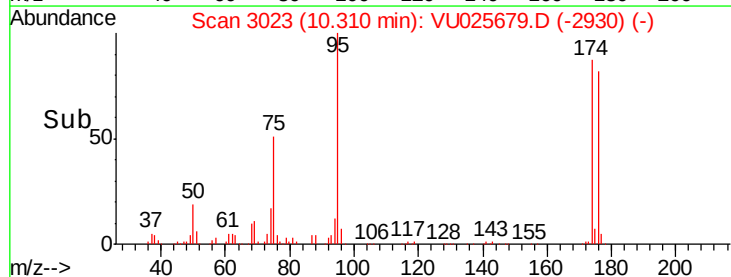
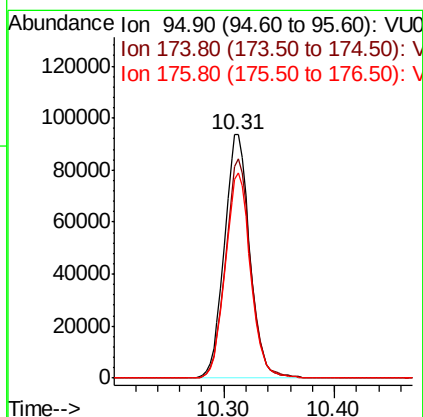
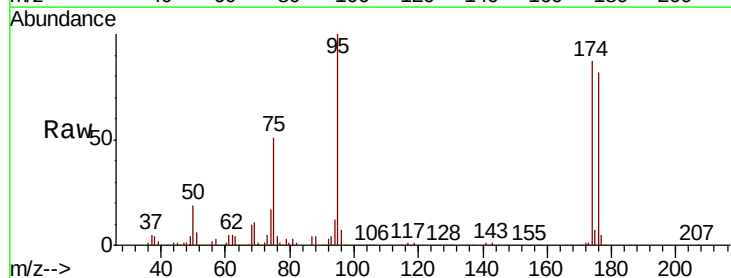


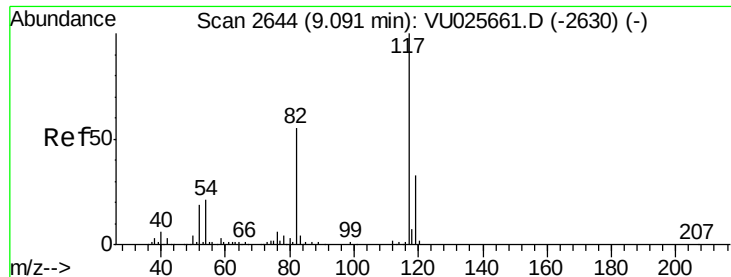

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 9.09 min Scan# 2645
Delta R.T. 0.00 min
Lab File: VU025679.D
Acq: 27 Jul 2018 19:13

Instrument :
MSVOA_U
ClientSampleId :
TB01-072518

Tot Ion:117 Resp: 262671
Ion Ratio Lower Upper
117 100
82 54.4 46.0 69.0
119 32.2 26.0 39.0

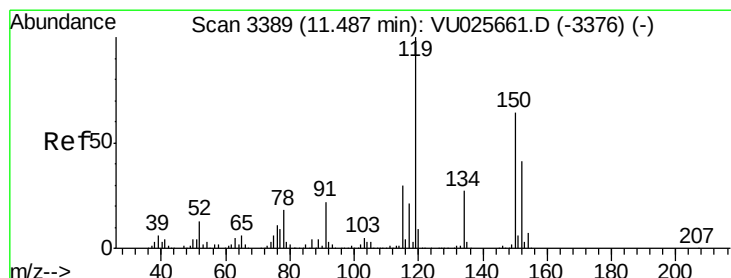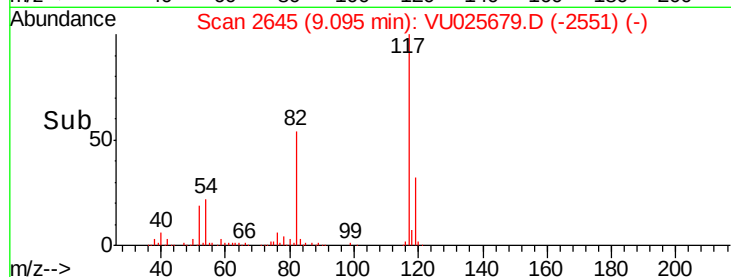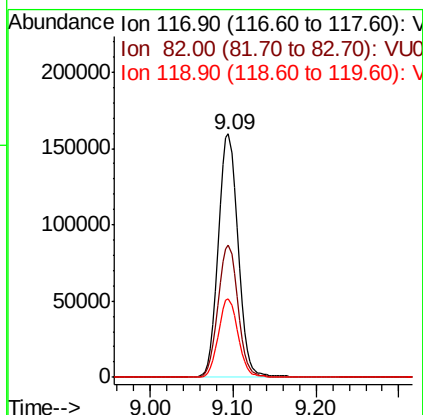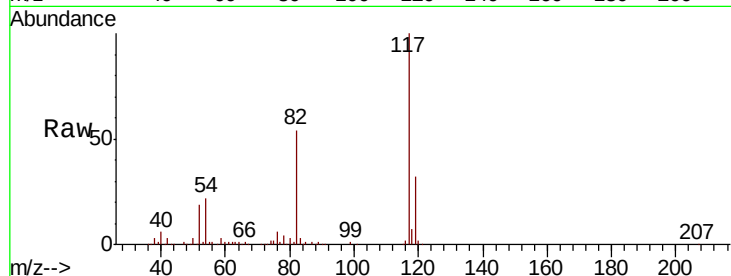

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 11.49 min Scan# 3389
Delta R.T. 0.00 min
Lab File: VU025679.D
Acq: 27 Jul 2018 19:13

Tgt Ion:152 Resp: 157959
Ion Ratio Lower Upper
152 100
115 56.6 40.1 120.3
150 154.3 0.0 351.4

