


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU072718\
Data File : VU025657.D
Acq On : 27 Jul 2018 08:59
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U072718W.M
Title : SW846 8260
Last Update : Tue Jul 31 16:07:47 2018

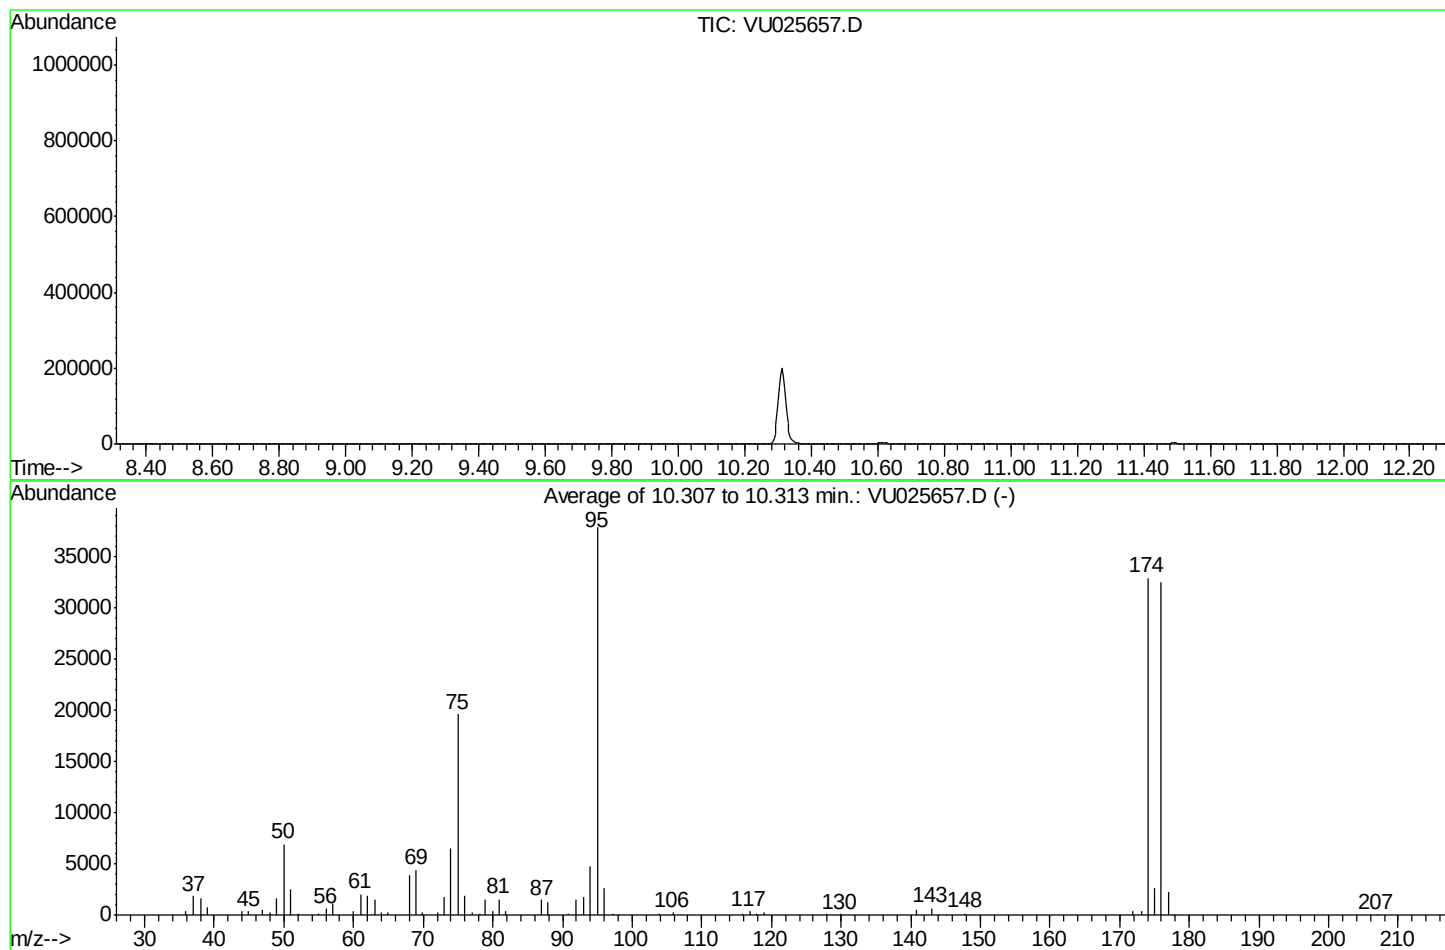

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3009

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	6915	PASS
75	95	30	60	51.8	19594	PASS
95	95	100	100	100.0	37850	PASS
96	95	5	9	6.9	2628	PASS
173	174	0.00	2	1.2	406	PASS
174	95	50	100	86.9	32874	PASS
175	174	5	9	7.9	2588	PASS
176	174	95	101	98.9	32504	PASS
177	176	5	9	6.9	2230	PASS