


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072718\
Data File : VU025683.D
Acq On : 27 Jul 2018 21:10
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U072718W.M
Title : SW846 8260
Last Update : Tue Jul 31 16:07:47 2018

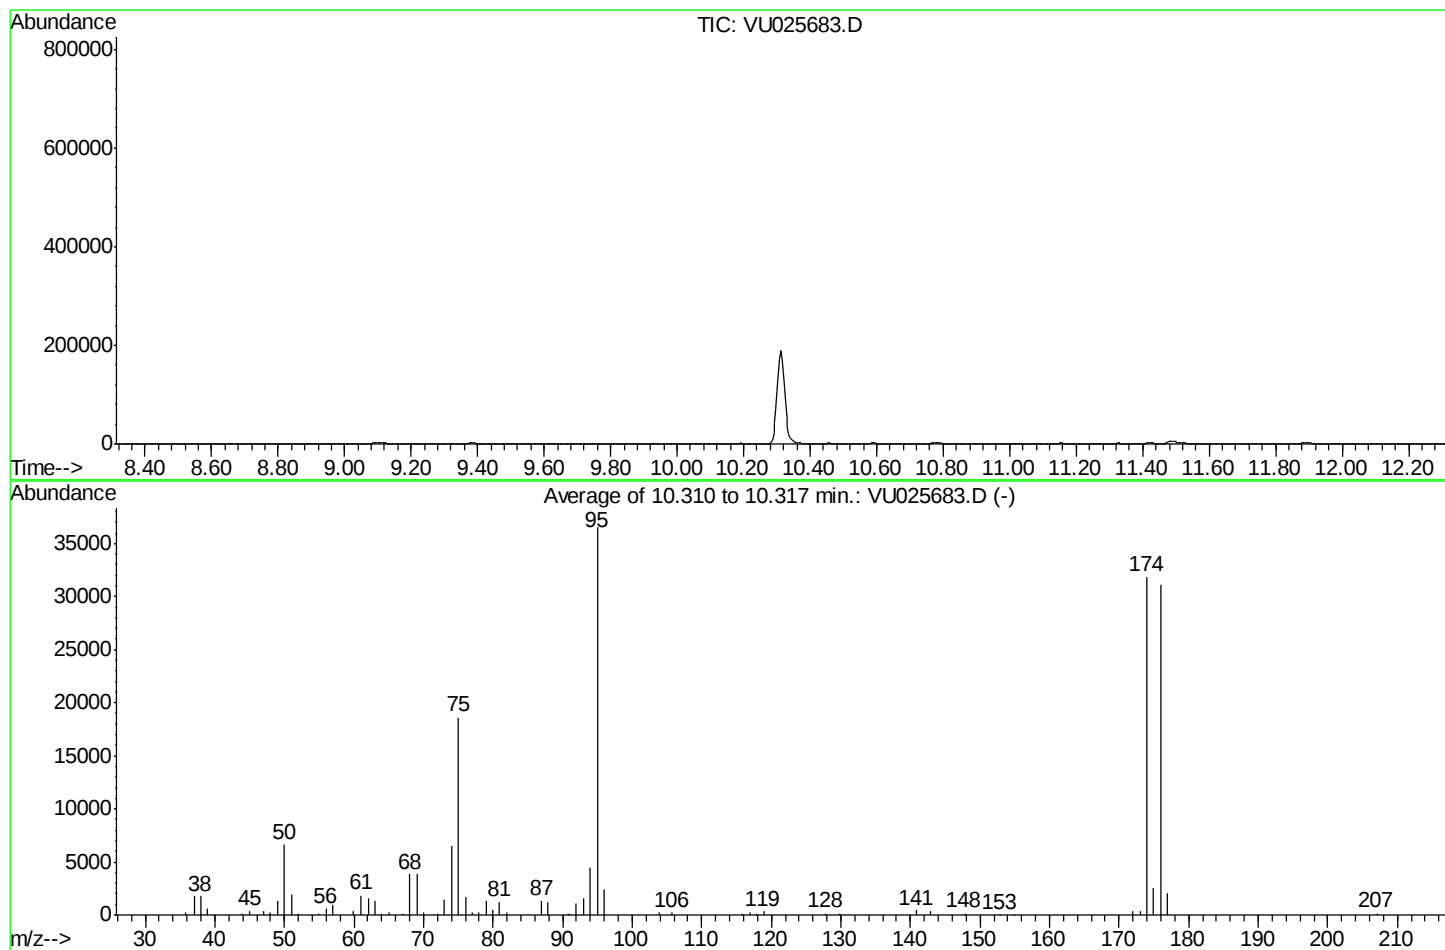

AutoFind: Scans 3023, 3024, 3025; Background Corrected with Scan 3010

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	6592	PASS
75	95	30	60	51.0	18618	PASS
95	95	100	100	100.0	36522	PASS
96	95	5	9	6.7	2458	PASS
173	174	0.00	2	1.3	406	PASS
174	95	50	100	87.3	31885	PASS
175	174	5	9	8.0	2539	PASS
176	174	95	101	97.6	31104	PASS
177	176	5	9	6.5	2012	PASS