

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072722\
 Data File : VU049976.D
 Acq On : 28 Jul 2022 03:34
 Operator : SY/MD
 Sample : N3922-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0C90

Quant Time: Jul 28 05:34:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jul 28 03:41:29 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	95490	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	93240	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	37255	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	39260	4.789	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.800%
7) Chloroethane-d5	1.913	69	31300	5.315	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	106.200%
11) 1,1-Dichloroethene-d2	2.565	65	14041	4.969	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	99.400%
20) 2-Butanone-d5	4.639	46	103280	56.589	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	113.180%
24) Chloroform-d	5.064	84	69163	5.098	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.000%
26) 1,2-Dichloroethane-d4	5.703	65	36242	5.301	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.000%
32) Benzene-d6	5.726	84	141179	5.124	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.400%
36) 1,2-Dichloropropane-d6	6.690	67	46831	5.188	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.800%
41) Toluene-d8	7.899	98	114843	4.690	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.800%
43) trans-1,3-Dichloroprop...	8.179	79	15299	4.836	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.800%
46) 2-Hexanone-d5	8.636	63	56460	47.676	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.360%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	40319	5.316	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	106.400%
66) 1,2-Dichlorobenzene-d4	12.195	152	38420	5.560	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.200%
Target Compounds						Qvalue
3) Chloromethane	1.520	50	2973	0.340	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072722\
Data File : VU049976.D
Acq On : 28 Jul 2022 03:34
Operator : SY/MD
Sample : N3922-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0C90


Quant Time: Jul 28 05:34:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jul 28 03:41:29 2022
Response via : Initial Calibration

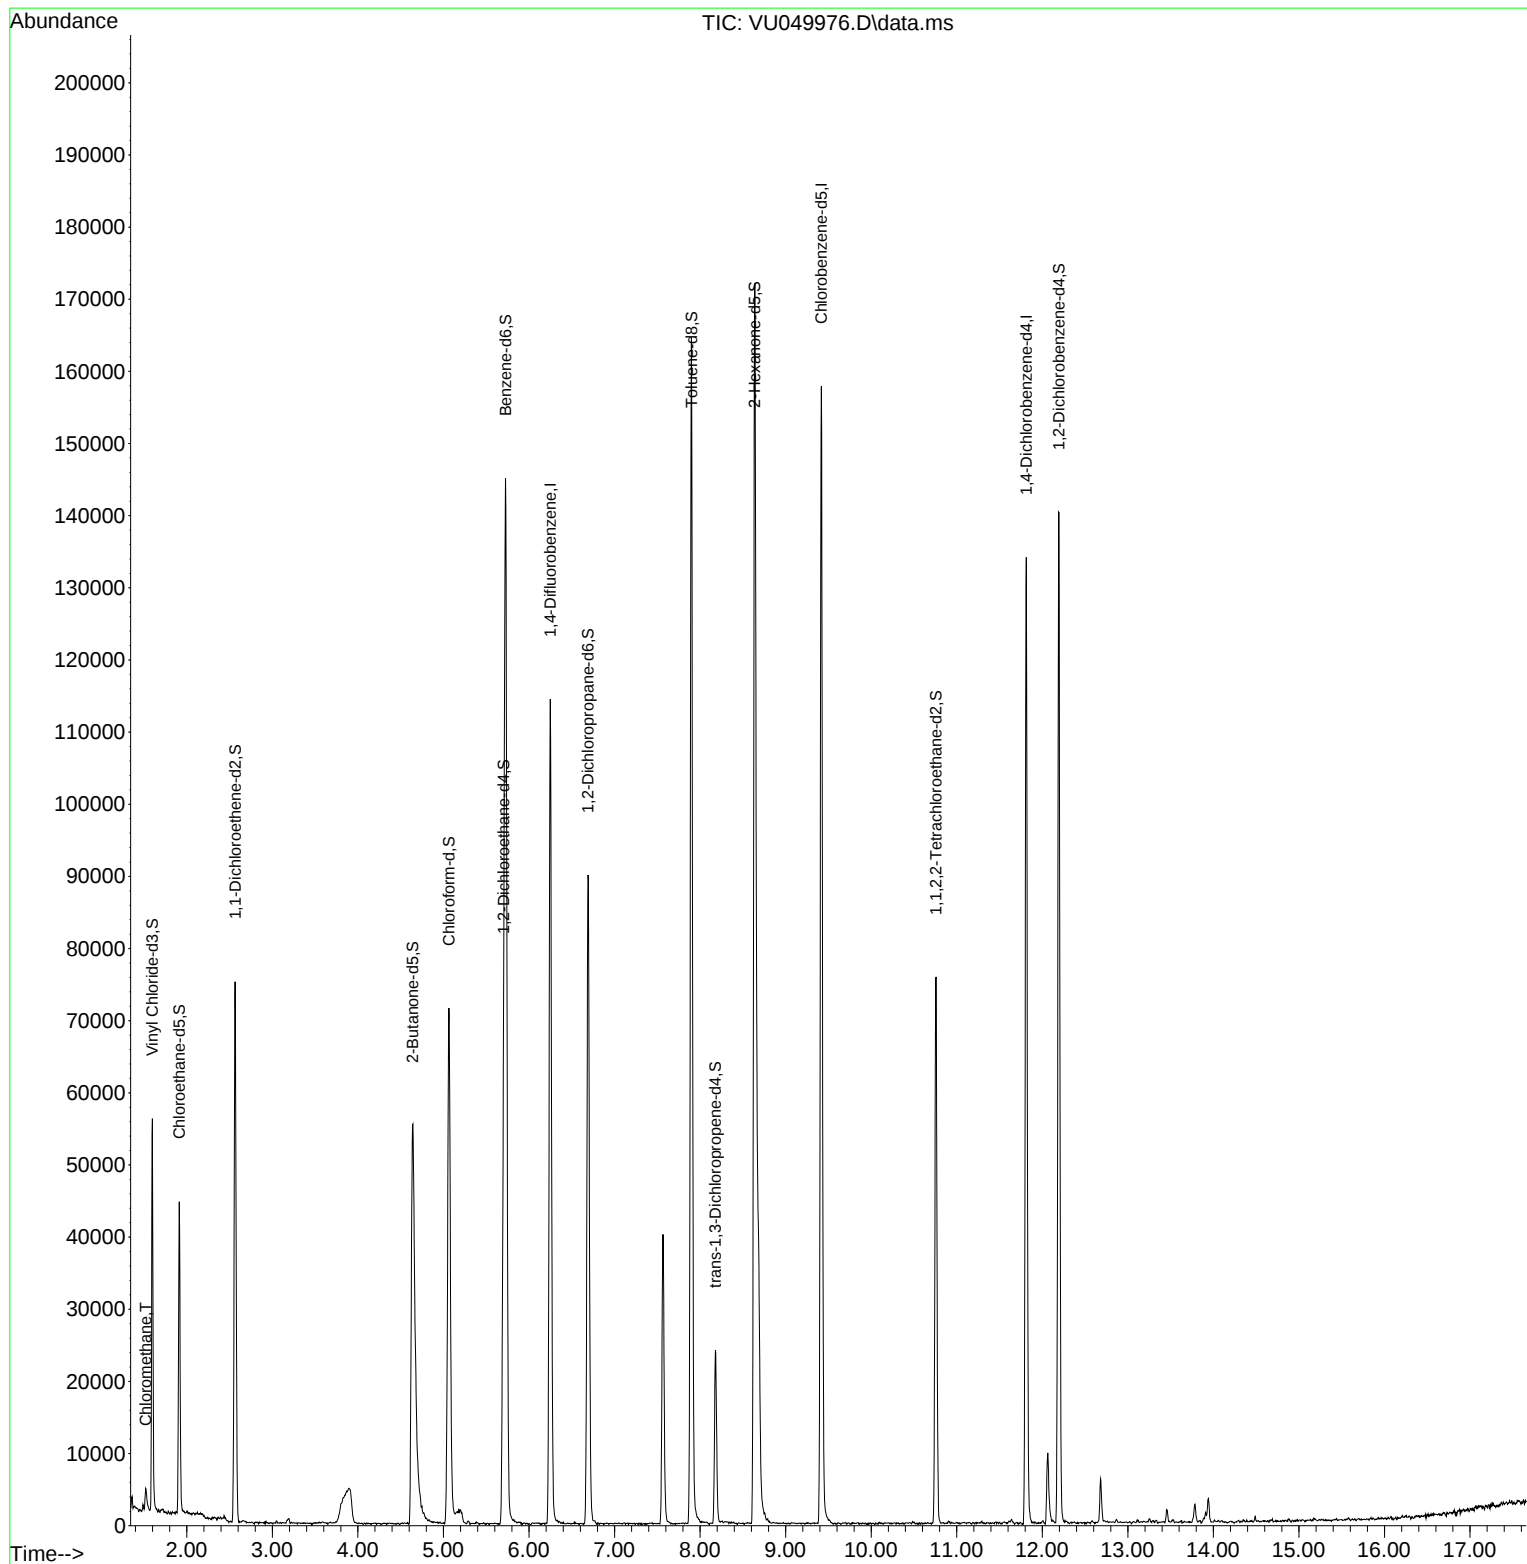

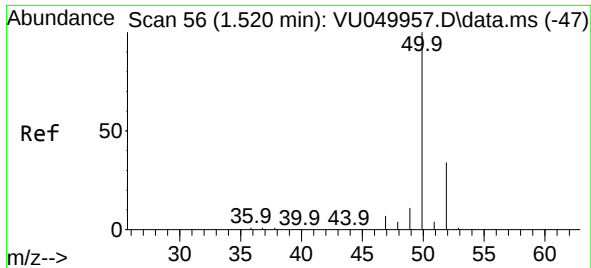

#3
 Chloromethane
 Concen: 0.340 ug/L
 RT: 1.520 min Scan# 50
 Delta R.T. 0.000 min
 Lab File: VU049976.D
 Acq: 28 Jul 2022 03:34

Instrument :
 MSVOA_U
 ClientSampleId :
 C0C90

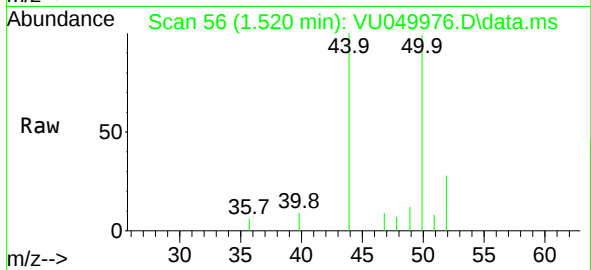

Tgt Ion: 50 Resp: 2973
 Ion Ratio Lower Upper
 50 100
 52 28.7 22.4 41.6

