

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072722\
 Data File : VU049977.D
 Acq On : 28 Jul 2022 03:59
 Operator : SY/MD
 Sample : N3922-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0C92

Quant Time: Jul 28 05:37:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jul 28 03:41:29 2022
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		6.250	114	92188	5.000	ug/L	0.00
28) Chlorobenzene-d5		9.417	117	92545	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.812	152	37098	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.597	65	39753	5.022	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	100.400%	
7) Chloroethane-d5		1.912	69	31827	5.598	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	112.000%	
11) 1,1-Dichloroethene-d2		2.565	65	14745	5.405	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	108.200%	
20) 2-Butanone-d5		4.636	46	102673	58.271	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	116.540%	
24) Chloroform-d		5.063	84	70620	5.392	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.800%	
26) 1,2-Dichloroethane-d4		5.703	65	36376	5.511	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.200%	
32) Benzene-d6		5.729	84	142110	5.197	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.000%	
36) 1,2-Dichloropropane-d6		6.690	67	48246	5.385	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.800%	
41) Toluene-d8		7.899	98	116999	4.813	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.200%	
43) trans-1,3-Dichloroprop...		8.179	79	14842	4.727	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.600%	
46) 2-Hexanone-d5		8.635	63	55442	47.168	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.340%	
56) 1,1,2,2-Tetrachloroeth...		10.758	84	40745	5.413	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.200%	
66) 1,2-Dichlorobenzene-d4		12.195	152	39591	5.754	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	115.000%	
Target Compounds							
						Qvalue	
3) Chloromethane		1.520	50	3935	0.467	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072722\
Data File : VU049977.D
Acq On : 28 Jul 2022 03:59
Operator : SY/MD
Sample : N3922-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0C92


Quant Time: Jul 28 05:37:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jul 28 03:41:29 2022
Response via : Initial Calibration

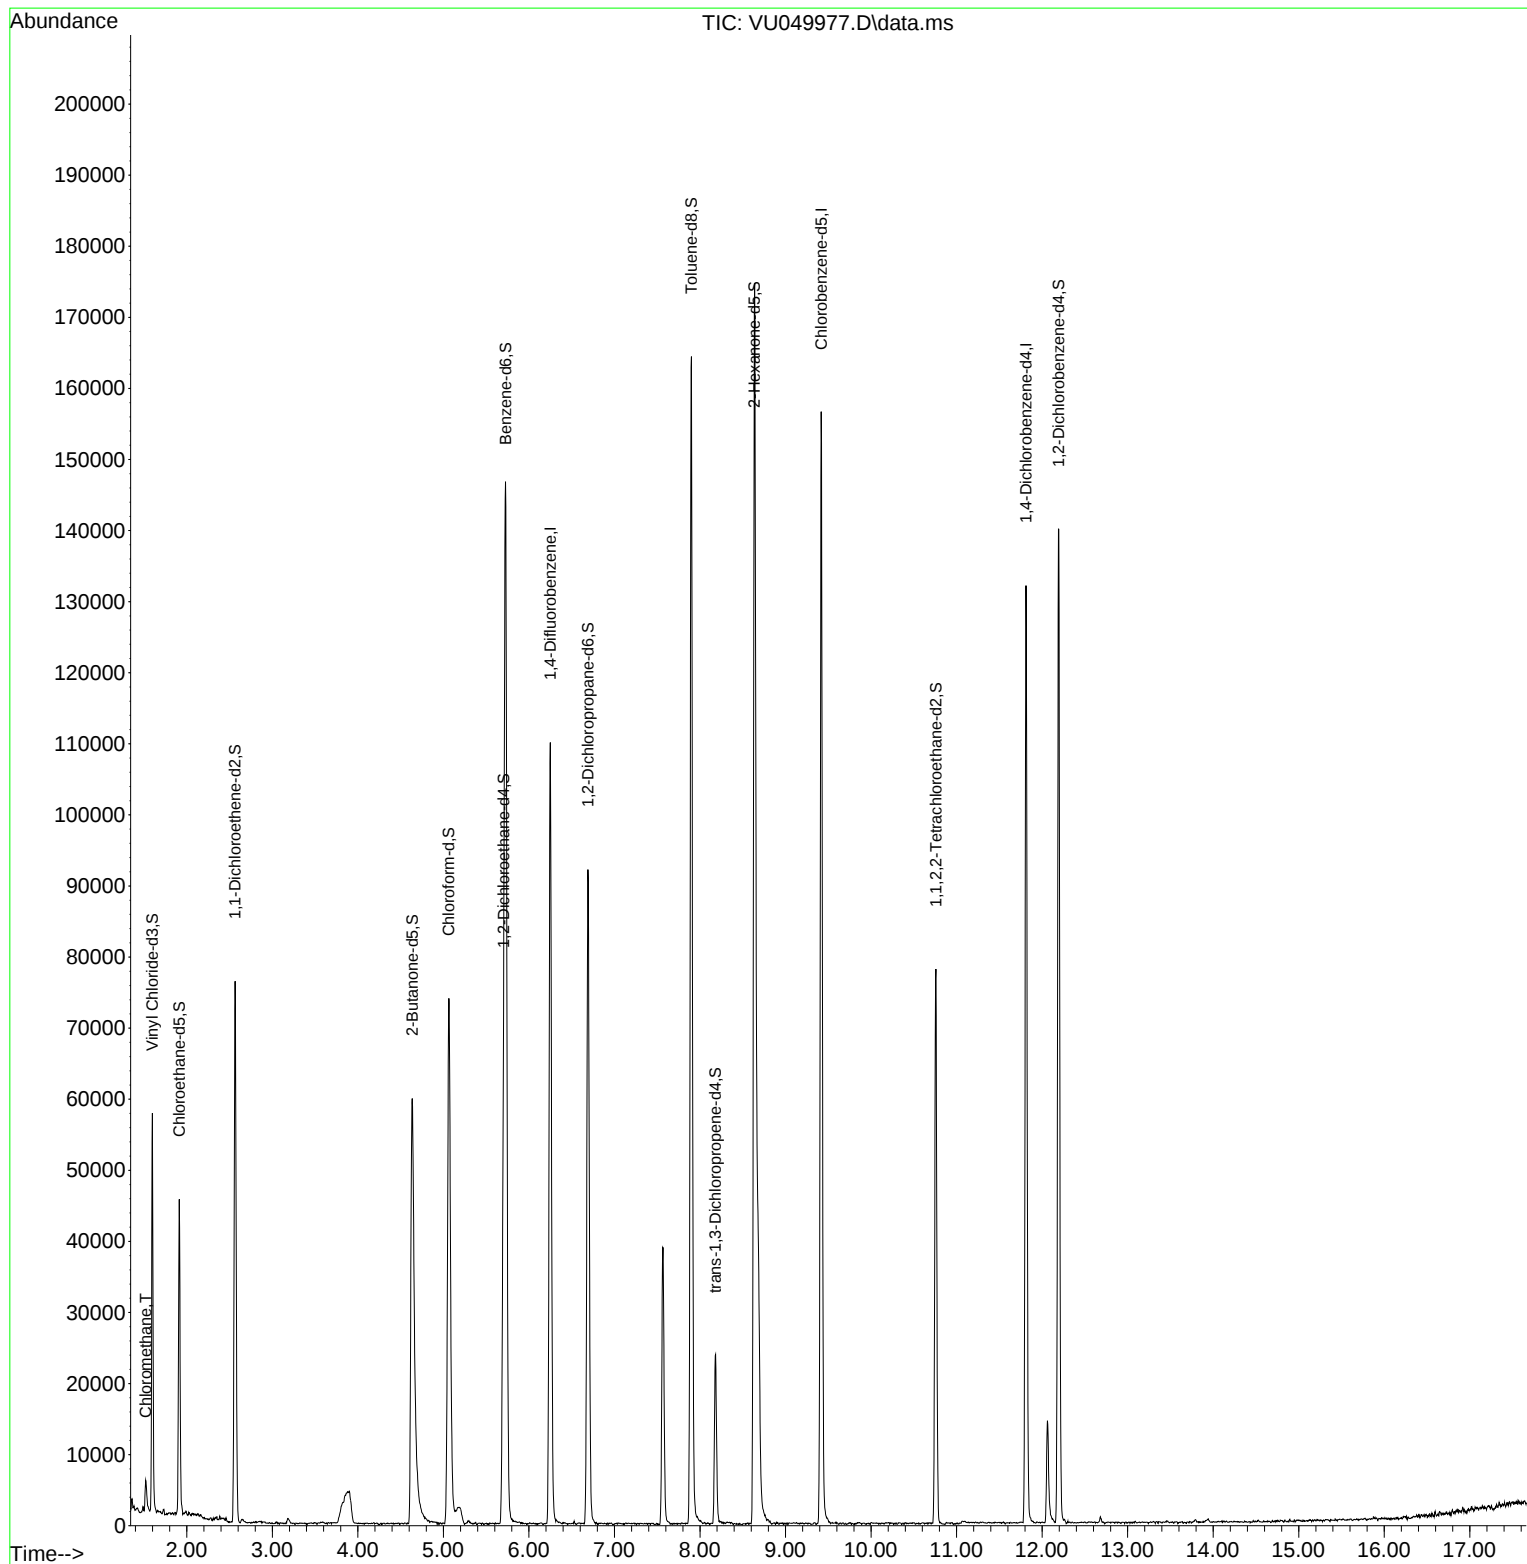

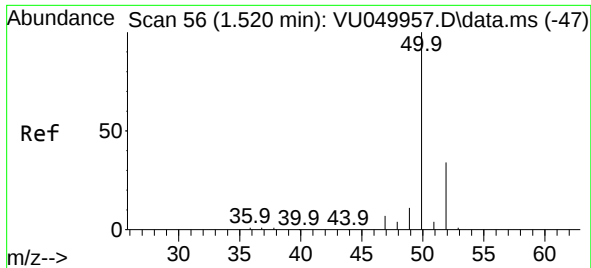

#3
 Chloromethane
 Concen: 0.467 ug/L
 RT: 1.520 min Scan# 50
 Delta R.T. -0.000 min
 Lab File: VU049977.D
 Acq: 28 Jul 2022 03:59

Instrument :
 MSVOA_U
 ClientSampleId :
 C0C92

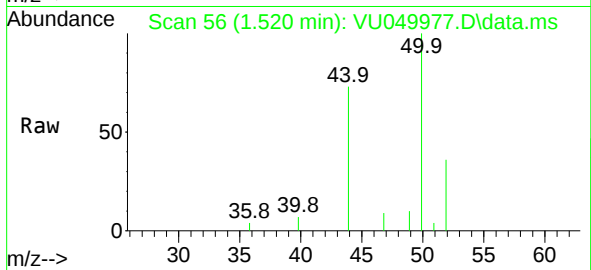

Tgt Ion: 50 Resp: 3935
 Ion Ratio Lower Upper
 50 100
 52 36.4 22.4 41.6

