

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072722\
 Data File : VU049958.D
 Acq On : 27 Jul 2022 20:07
 Operator : SY/MD
 Sample : VU0727WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK100

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU049958.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.594	72	79	93	rVB	57482	64764	15.26%	2.112%
2	1.909	170	177	192	rVB	45510	57835	13.62%	1.886%
3	2.565	369	381	396	rVB	77116	124069	29.23%	4.047%
4	3.044	521	530	547	rVB3	5636	10689	2.52%	0.349%
5	3.186	558	574	586	rBV	5984	13554	3.19%	0.442%
6	3.851	750	781	783	rBV	2967	10225	2.41%	0.333%
7	4.645	1013	1028	1070	rBV2	55125	201002	47.35%	6.556%
8	5.063	1142	1158	1178	rBV	72692	161885	38.13%	5.280%
9	5.726	1344	1364	1386	rBV3	149363	380121	89.54%	12.398%
10	6.250	1514	1527	1552	rBV	112742	214517	50.53%	6.997%
11	6.690	1650	1664	1685	rBV	92005	178783	42.11%	5.831%
12	7.568	1926	1937	1955	rBV	42315	74692	17.59%	2.436%
13	7.899	2026	2040	2054	rBV	161924	283746	66.84%	9.255%
14	7.970	2057	2062	2075	rVB2	3271	5494	1.29%	0.179%
15	8.182	2114	2128	2141	rBV	25945	44528	10.49%	1.452%
16	8.639	2257	2270	2308	rBV4	174106	424524	100.00%	13.846%
17	9.417	2500	2512	2533	rBV	158941	267291	62.96%	8.718%
18	10.758	2917	2929	2947	rBV	77411	122630	28.89%	4.000%
19	11.812	3243	3257	3277	rBV	128841	209018	49.24%	6.817%
20	12.195	3364	3376	3397	rBV	132216	216664	51.04%	7.067%




Sum of corrected areas: 3066031

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072722\
Data File : VU049958.D
Acq On : 27 Jul 2022 20:07
Operator : SY/MD
Sample : VU0727WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK100

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

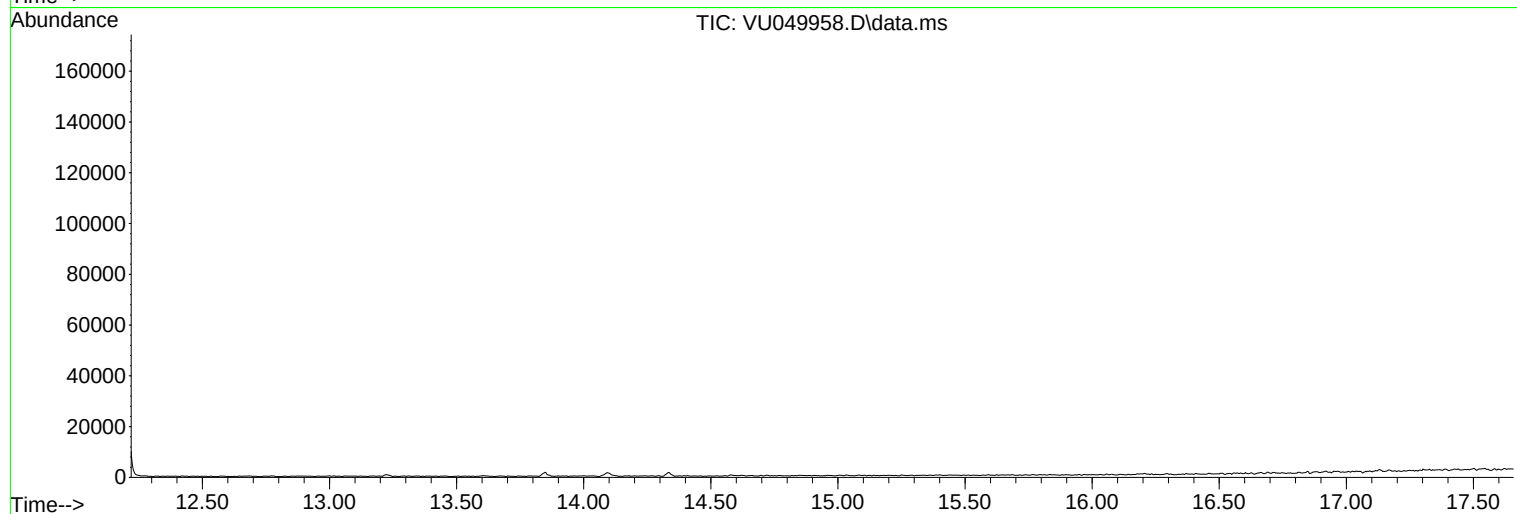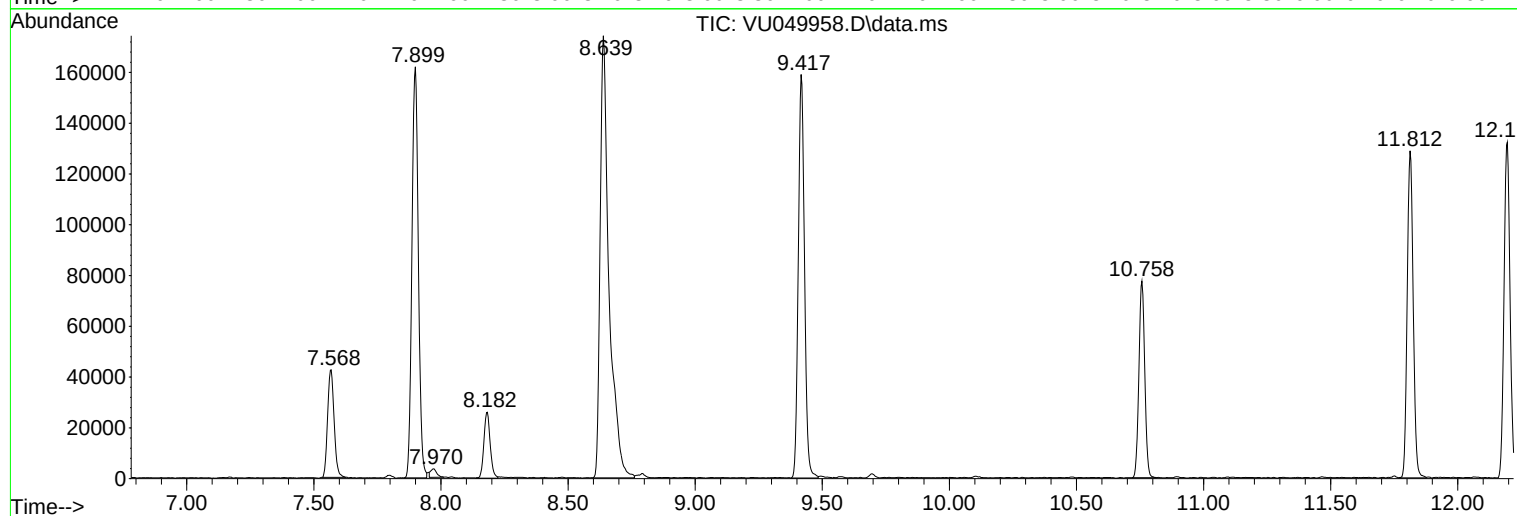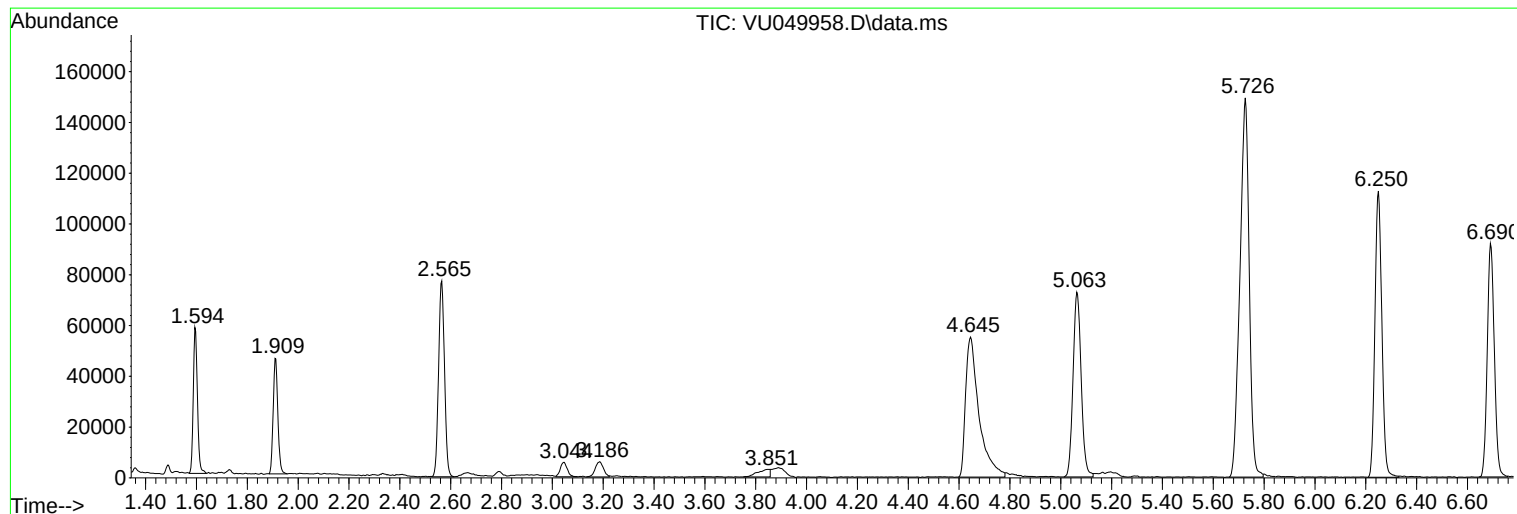

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072722\
Data File : VU049958.D
Acq On : 27 Jul 2022 20:07
Operator : SY/MD
Sample : VU0727WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK100

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072722\
Data File : VU049958.D
Acq On : 27 Jul 2022 20:07
Operator : SY/MD
Sample : VU0727WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK100

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc