

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072722\
 Data File : VU049959.D
 Acq On : 27 Jul 2022 20:39
 Operator : SY/MD
 Sample : N3873-09
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBJ33

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU049959.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.481	37	44	49	rBV	17881	17428	1.81%	0.132%
2	1.520	49	56	71	rVV	34225	58467	6.08%	0.443%
3	1.597	72	80	97	rVB	61200	71597	7.44%	0.542%
4	1.858	154	161	170	rVV	36708	48198	5.01%	0.365%
5	1.912	170	178	194	rVB	46448	60239	6.26%	0.456%
6	2.134	234	247	263	rVB	136131	198470	20.63%	1.503%
7	2.568	369	382	395	rBV3	132220	254909	26.50%	1.930%
8	2.645	395	406	429	rBV	29848	89517	9.31%	0.678%
9	2.784	439	449	470	rVB	79032	138481	14.40%	1.048%
10	3.041	517	529	547	rBV	50241	92801	9.65%	0.703%
11	3.372	613	632	655	rBV	144860	337774	35.11%	2.557%
12	3.861	767	784	810	rVB	110756	267490	27.81%	2.025%
13	4.658	1018	1032	1044	rBV	43122	123147	12.80%	0.932%
14	4.732	1044	1055	1120	rVB	110713	440041	45.74%	3.332%
15	5.063	1143	1158	1176	rBV	74159	162489	16.89%	1.230%
16	5.311	1218	1235	1245	rBV	135713	303777	31.58%	2.300%
17	5.378	1245	1256	1276	rVB2	240149	538460	55.98%	4.077%
18	5.722	1345	1363	1376	rBV2	163113	387331	40.26%	2.932%
19	5.796	1376	1386	1406	rVB	72955	149661	15.56%	1.133%
20	6.250	1514	1527	1545	rBV	120988	225977	23.49%	1.711%
21	6.539	1604	1617	1641	rBV	114366	216223	22.48%	1.637%
22	6.693	1651	1665	1674	rBV	91690	177195	18.42%	1.342%
23	6.758	1674	1685	1717	rVB2	178803	435577	45.28%	3.298%
24	7.568	1925	1937	1956	rBV	44590	78628	8.17%	0.595%
25	7.899	2027	2040	2051	rBV	176735	304116	31.61%	2.302%
26	7.970	2051	2062	2090	rVB	372183	629028	65.39%	4.762%
27	8.182	2117	2128	2143	rBV	27622	46496	4.83%	0.352%
28	8.552	2230	2243	2259	rBV	219168	367136	38.17%	2.780%
29	8.645	2259	2272	2279	rVV2	176690	358585	37.28%	2.715%
30	8.690	2279	2286	2331	rVB	313669	636125	66.13%	4.816%
31	8.925	2345	2359	2381	rBV	134582	237961	24.74%	1.802%
32	9.446	2499	2521	2538	rBV2	404969	937188	97.42%	7.095%
33	9.536	2538	2549	2553	rVV	145530	235038	24.43%	1.779%
34	9.571	2553	2560	2583	rVV	312117	505993	52.60%	3.831%
35	9.697	2586	2599	2628	rVB	616515	961959	100.00%	7.283%
36	10.108	2712	2727	2755	rBV3	365941	745394	77.49%	5.643%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072722\
 Data File : VU049959.D
 Acq On : 27 Jul 2022 20:39
 Operator : SY/MD
 Sample : N3873-09
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBJ33

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
 Title : TRACE VOA SFAM1.0

37	10.291	2772	2784	2802	rVB	46763	78116	8.12%	0.591%
38	10.484	2832	2844	2857	rBV	164414	253947	26.40%	1.923%
39	10.758	2918	2929	2944	rVB	80217	126849	13.19%	0.960%
40	11.815	3246	3258	3261	rBV	170673	262860	27.33%	1.990%
41	12.211	3362	3381	3403	rBV2	454412	926350	96.30%	7.013%
42	12.999	3614	3626	3636	rBV2	17556	27860	2.90%	0.211%
43	13.220	3683	3695	3711	rBV	174125	274607	28.55%	2.079%
44	14.330	4024	4040	4060	rBV	267106	418966	43.55%	3.172%




Sum of corrected areas: 13208451

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072722\
Data File : VU049959.D
Acq On : 27 Jul 2022 20:39
Operator : SY/MD
Sample : N3873-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBJ33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

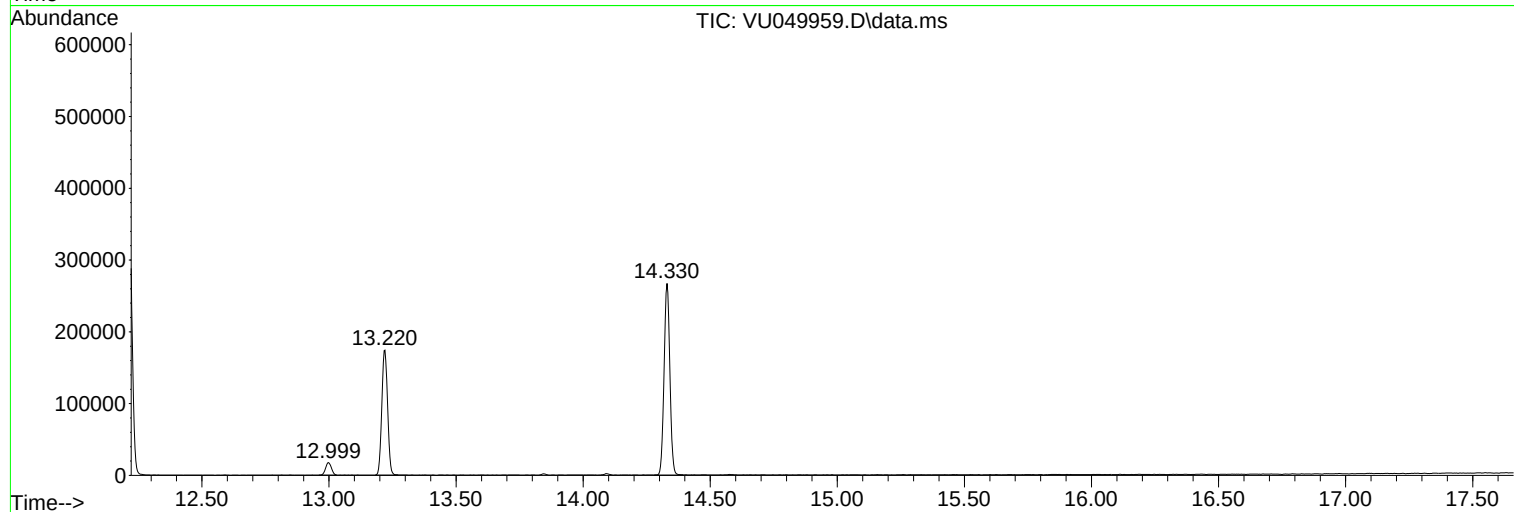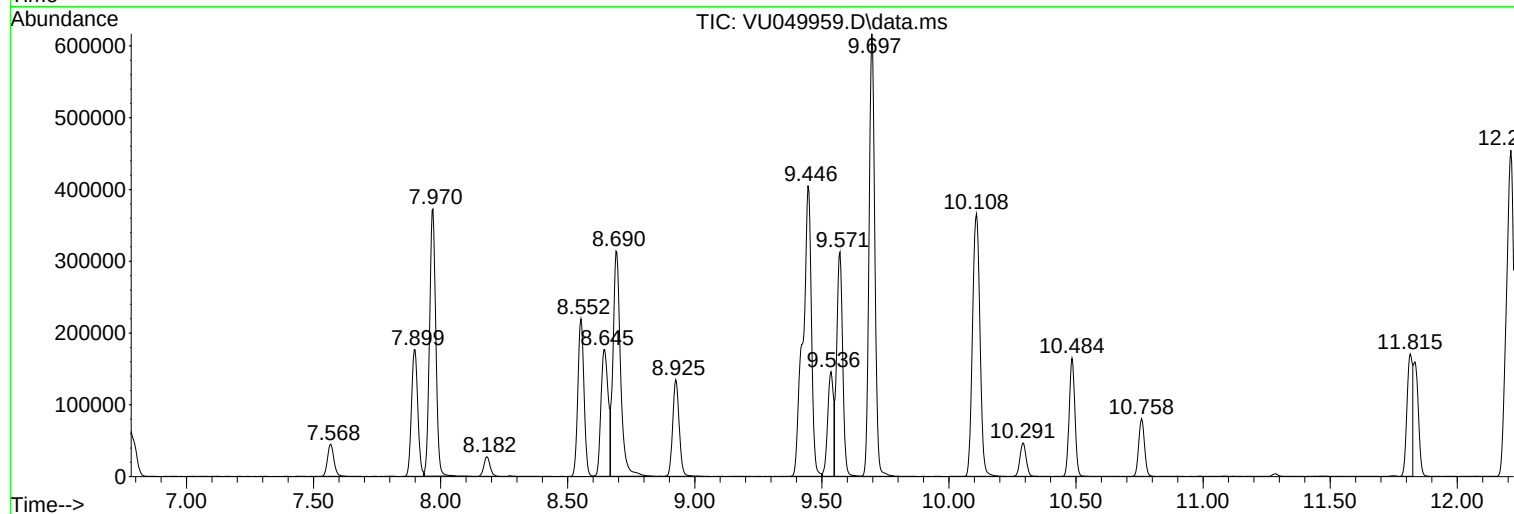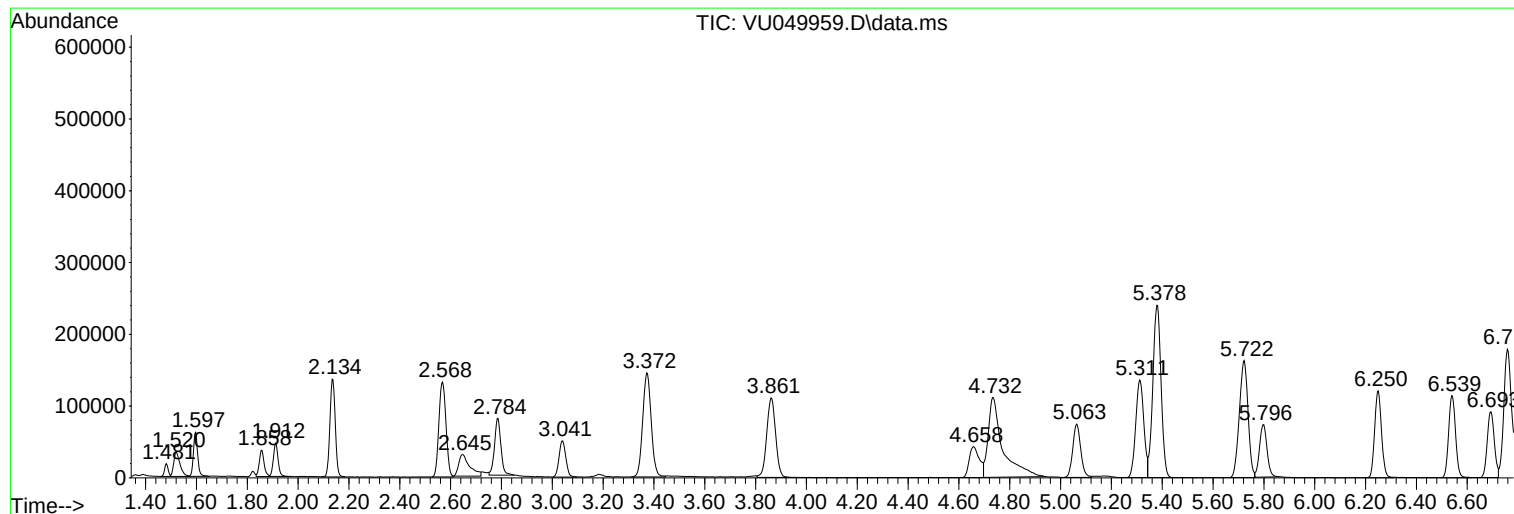

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072722\
Data File : VU049959.D
Acq On : 27 Jul 2022 20:39
Operator : SY/MD
Sample : N3873-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBJ33










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Benzene, 1,3,5-trichloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.220	5.22 ug/L	274607	1,4-Dichlorobenzene-d4	11.812

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1,3,5-trichloro-	180	C6H3Cl3	000108-70-3	98
2			Benzene, 1,2,3-trichloro-	180	C6H3Cl3	000087-61-6	98
3			Benzene, 1,3,5-trichloro-	180	C6H3Cl3	000108-70-3	97
4			Benzene, 1,3,5-trichloro-	180	C6H3Cl3	000108-70-3	97
5			Benzene, 1,2,4-trichloro-	180	C6H3Cl3	000120-82-1	97

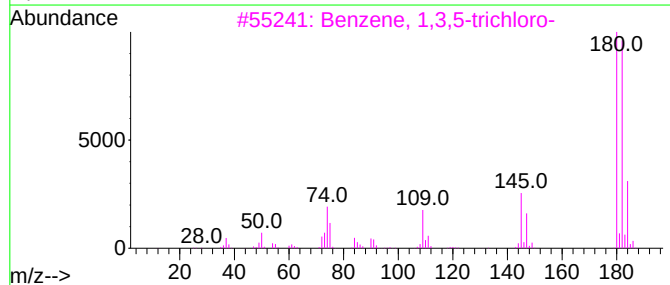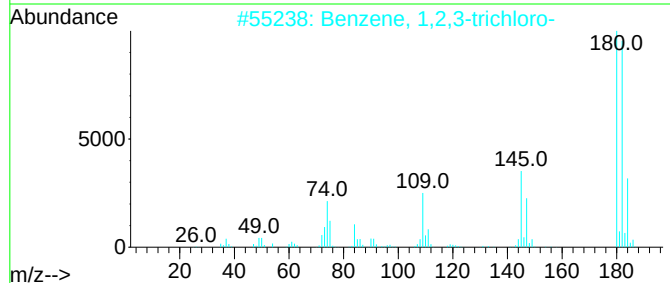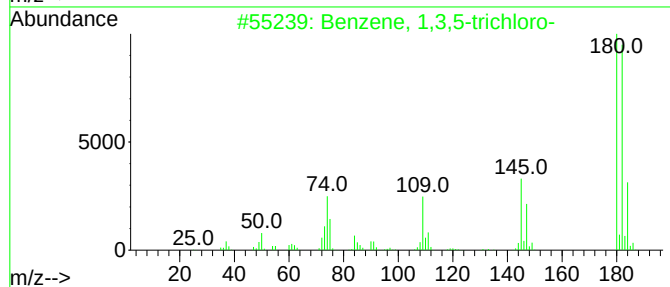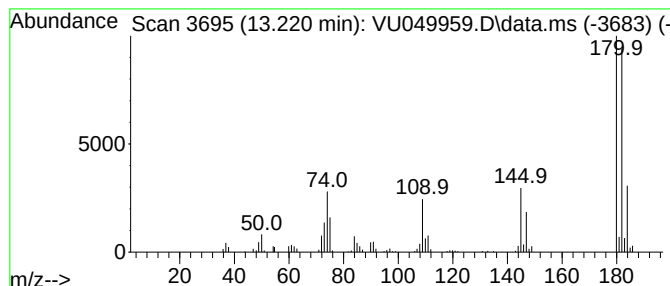

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072722\
Data File : VU049959.D
Acq On : 27 Jul 2022 20:39
Operator : SY/MD
Sample : N3873-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBJ33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzene, 1,3,5-...	13.220	5.2	ug/L	274607	3	11.812	262860	5.0