

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072722\
 Data File : VU049966.D
 Acq On : 27 Jul 2022 23:29
 Operator : SY/MD
 Sample : N3870-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBJ01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU049966.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.594	72	79	101	rBV	56010	64250	11.23%	1.546%
2	1.912	169	178	190	rBV	41962	53715	9.39%	1.293%
3	2.369	310	320	331	rBV	7945	12638	2.21%	0.304%
4	2.575	369	384	401	rVB2	243474	497142	86.90%	11.966%
5	3.796	744	764	768	rBV	2437	5987	1.05%	0.144%
6	4.661	1013	1033	1076	rBV3	73627	272025	47.55%	6.547%
7	5.063	1140	1158	1178	rBV	70504	155350	27.15%	3.739%
8	5.726	1344	1364	1391	rBV2	142939	365143	63.82%	8.789%
9	6.250	1514	1527	1551	rBV	103008	197414	34.51%	4.752%
10	6.542	1603	1618	1639	rBV	304920	572110	100.00%	13.770%
11	6.690	1651	1664	1683	rVB2	86310	171314	29.94%	4.123%
12	7.568	1924	1937	1958	rBV	40489	71703	12.53%	1.726%
13	7.899	2026	2040	2056	rBV	159277	279653	48.88%	6.731%
14	8.182	2117	2128	2141	rBV2	23934	40911	7.15%	0.985%
15	8.552	2231	2243	2258	rBV2	112551	189787	33.17%	4.568%
16	8.639	2258	2270	2305	rVV3	170931	426707	74.58%	10.270%
17	9.417	2500	2512	2531	rBV	148884	245942	42.99%	5.920%
18	10.758	2915	2929	2946	rBV	73513	119333	20.86%	2.872%
19	11.812	3246	3257	3273	rBV	123604	196451	34.34%	4.728%
20	12.192	3364	3375	3396	rBV	133003	217148	37.96%	5.227%




Sum of corrected areas: 4154723

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072722\
Data File : VU049966.D
Acq On : 27 Jul 2022 23:29
Operator : SY/MD
Sample : N3870-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBJ01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

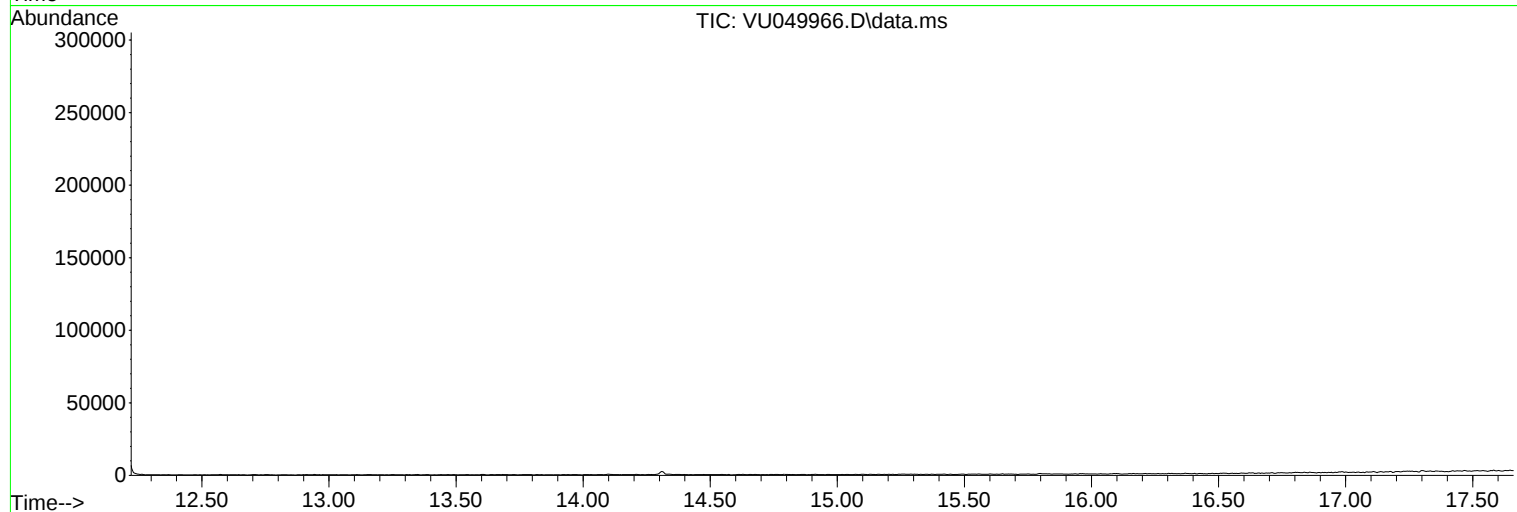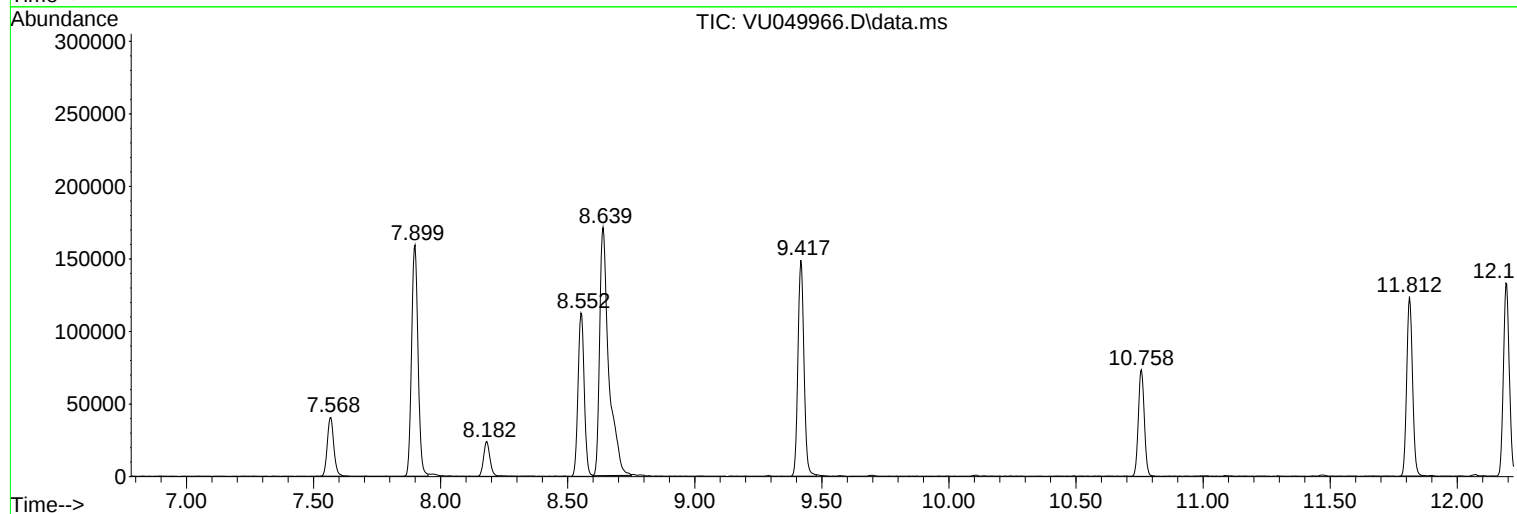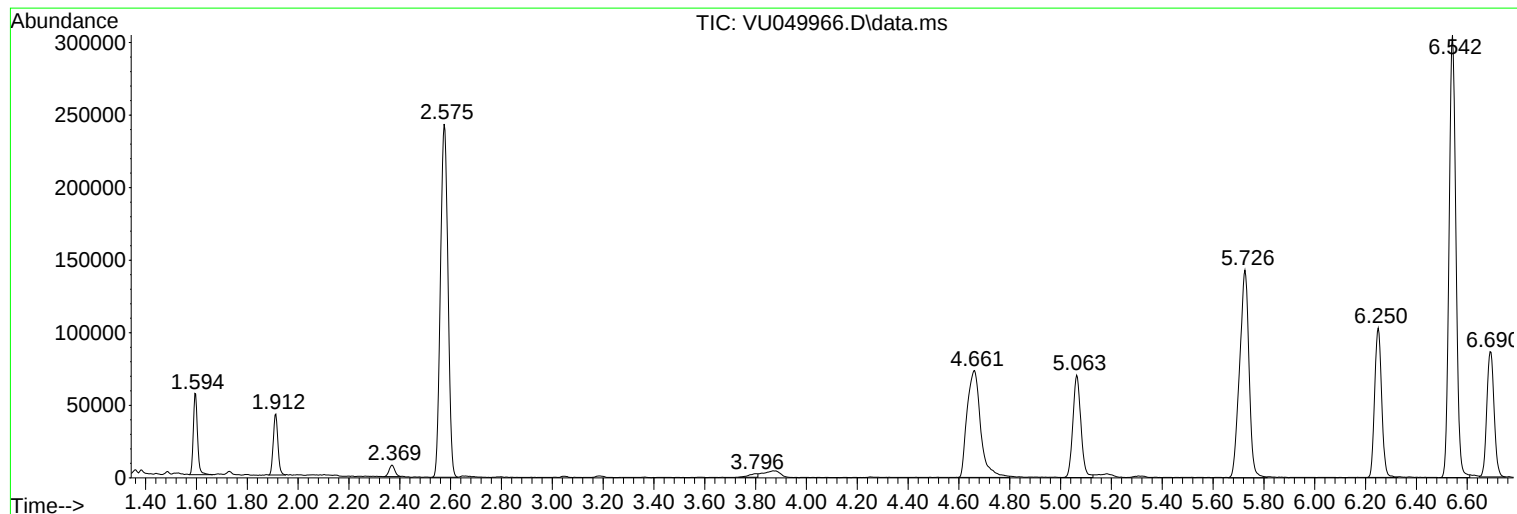

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072722\
Data File : VU049966.D
Acq On : 27 Jul 2022 23:29
Operator : SY/MD
Sample : N3870-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBJ01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072722\
Data File : VU049966.D
Acq On : 27 Jul 2022 23:29
Operator : SY/MD
Sample : N3870-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBJ01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
