

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072722\
 Data File : VU049969.D
 Acq On : 28 Jul 2022 00:42
 Operator : SY/MD
 Sample : N3922-19
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CB3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU049969.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	98	rVB	62970	71831	16.51%	2.286%
2	1.912	170	178	193	rVB	46806	60377	13.88%	1.922%
3	2.565	367	381	397	rBV	86933	139910	32.15%	4.453%
4	3.877	758	789	790	rBV	4287	14726	3.38%	0.469%
5	4.636	1012	1025	1064	rBV	58940	176696	40.61%	5.623%
6	5.063	1143	1158	1186	rBV	77868	175247	40.28%	5.577%
7	5.726	1340	1364	1388	rBV2	154732	393012	90.32%	12.508%
8	6.250	1513	1527	1545	rBV	108103	207226	47.63%	6.595%
9	6.690	1651	1664	1684	rBV2	94474	184354	42.37%	5.867%
10	7.565	1922	1936	1954	rBV	42366	74518	17.13%	2.372%
11	7.899	2024	2040	2058	rBV	174418	307631	70.70%	9.791%
12	8.182	2117	2128	2142	rBV2	25094	42692	9.81%	1.359%
13	8.639	2256	2270	2308	rBV5	175379	435120	100.00%	13.848%
14	8.790	2308	2317	2325	rVB4	4885	8252	1.90%	0.263%
15	9.417	2500	2512	2534	rBV	153412	257064	59.08%	8.181%
16	10.118	2718	2730	2745	rBV2	5519	9244	2.12%	0.294%
17	10.758	2913	2929	2945	rBV	77344	124447	28.60%	3.961%
18	11.478	3145	3153	3166	rBV3	3273	6231	1.43%	0.198%
19	11.812	3246	3257	3279	rBV	132014	208571	47.93%	6.638%
20	12.063	3328	3335	3346	rBV4	4552	7891	1.81%	0.251%
21	12.192	3364	3375	3399	rBV	144053	237067	54.48%	7.545%




Sum of corrected areas: 3142107

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072722\
Data File : VU049969.D
Acq On : 28 Jul 2022 00:42
Operator : SY/MD
Sample : N3922-19
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

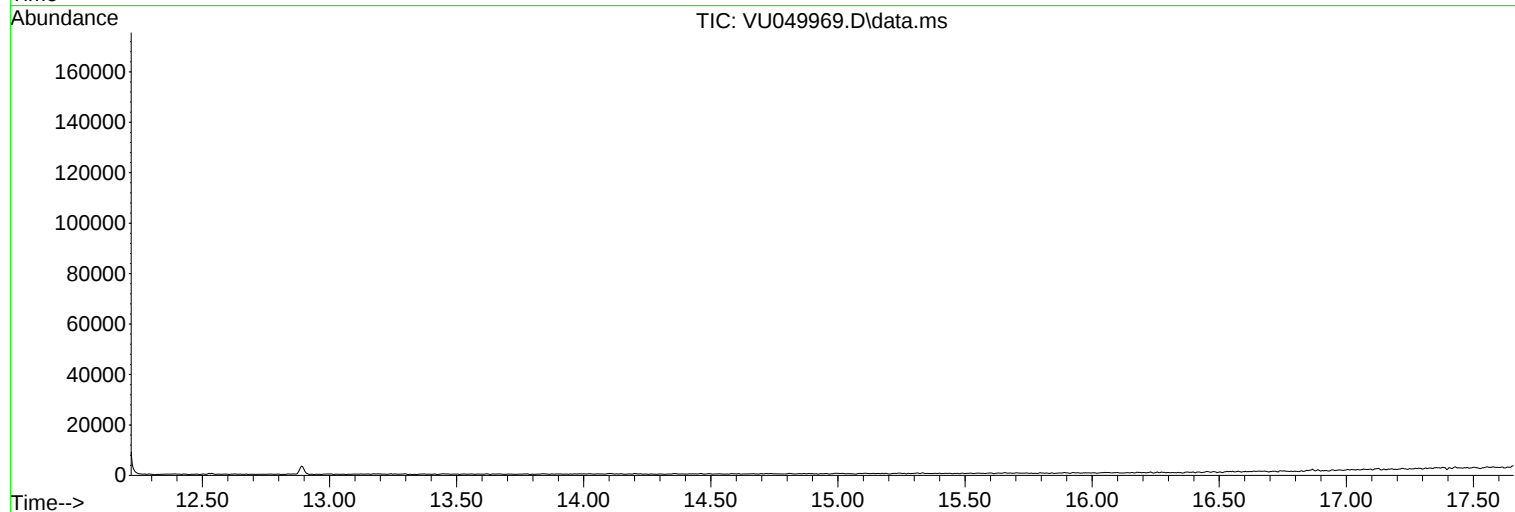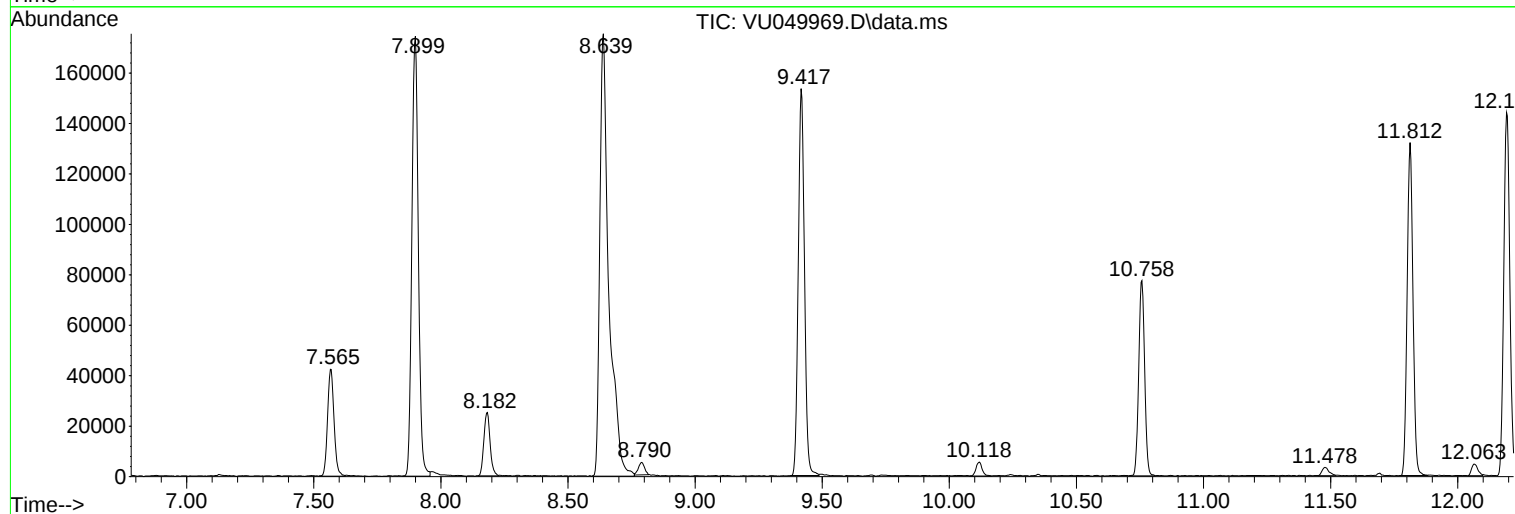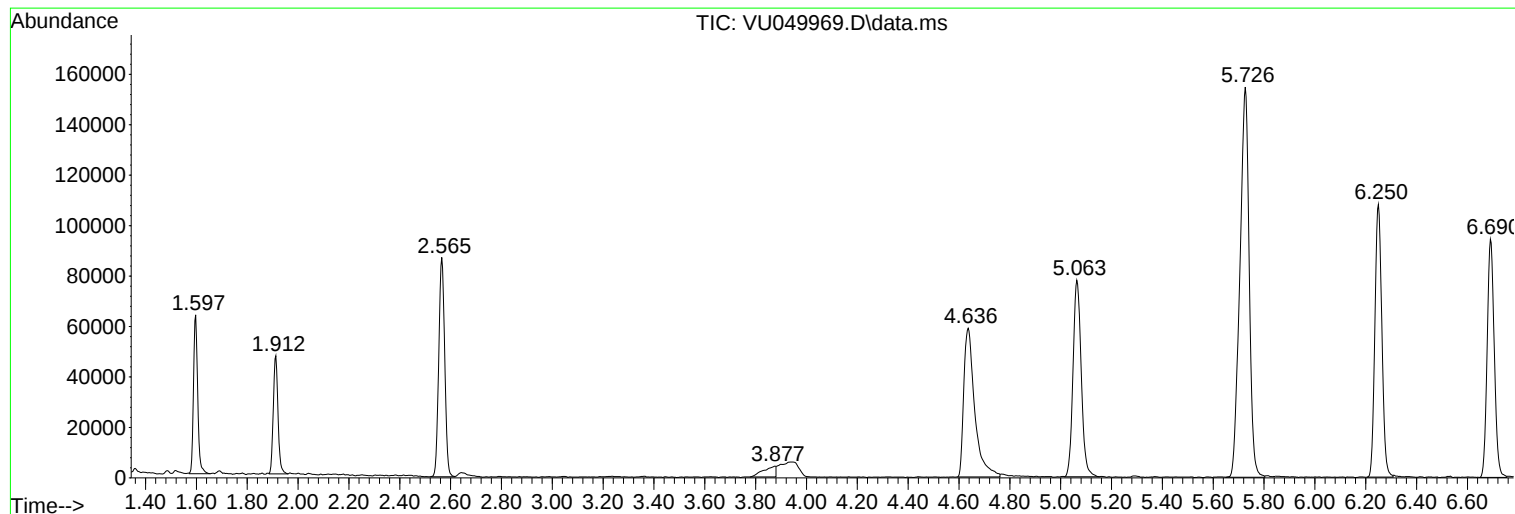

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072722\
Data File : VU049969.D
Acq On : 28 Jul 2022 00:42
Operator : SY/MD
Sample : N3922-19
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072722\
Data File : VU049969.D
Acq On : 28 Jul 2022 00:42
Operator : SY/MD
Sample : N3922-19
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc