

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072722\
 Data File : VU049976.D
 Acq On : 28 Jul 2022 03:34
 Operator : SY/MD
 Sample : N3922-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0C90

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049976.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.520	50	56	71	rVB2	3026	4771	1.11%	0.157%
2	1.597	72	80	94	rBV	54250	60277	13.98%	1.982%
3	1.913	170	178	189	rBV	43151	54299	12.59%	1.785%
4	2.565	369	381	395	rBV	74932	118977	27.59%	3.911%
5	3.829	750	774	776	rBV	3402	9368	2.17%	0.308%
6	4.642	1012	1027	1058	rBV	55474	179579	41.64%	5.904%
7	5.064	1143	1158	1181	rBV	71427	162389	37.65%	5.338%
8	5.726	1343	1364	1392	rBV2	144947	372636	86.40%	12.250%
9	6.250	1514	1527	1548	rBV	114259	213819	49.57%	7.029%
10	6.690	1650	1664	1684	rBV	89889	175163	40.61%	5.758%
11	7.565	1925	1936	1953	rBV	40127	70647	16.38%	2.322%
12	7.899	2027	2040	2061	rBV	164355	288304	66.84%	9.478%
13	8.179	2116	2127	2145	rBV	24001	40404	9.37%	1.328%
14	8.639	2258	2270	2304	rBV4	171840	431305	100.00%	14.179%
15	9.417	2500	2512	2538	rBV	157617	265977	61.67%	8.744%
16	10.758	2917	2929	2946	rVB	75726	121996	28.29%	4.011%
17	11.812	3246	3257	3276	rBV	133957	215691	50.01%	7.091%
18	12.063	3326	3335	3350	rBV2	9879	17995	4.17%	0.592%
19	12.192	3364	3375	3396	rBV	140120	229130	53.12%	7.533%
20	12.681	3515	3527	3538	rBV3	6064	9142	2.12%	0.301%




Sum of corrected areas: 3041869

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072722\
Data File : VU049976.D
Acq On : 28 Jul 2022 03:34
Operator : SY/MD
Sample : N3922-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0C90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

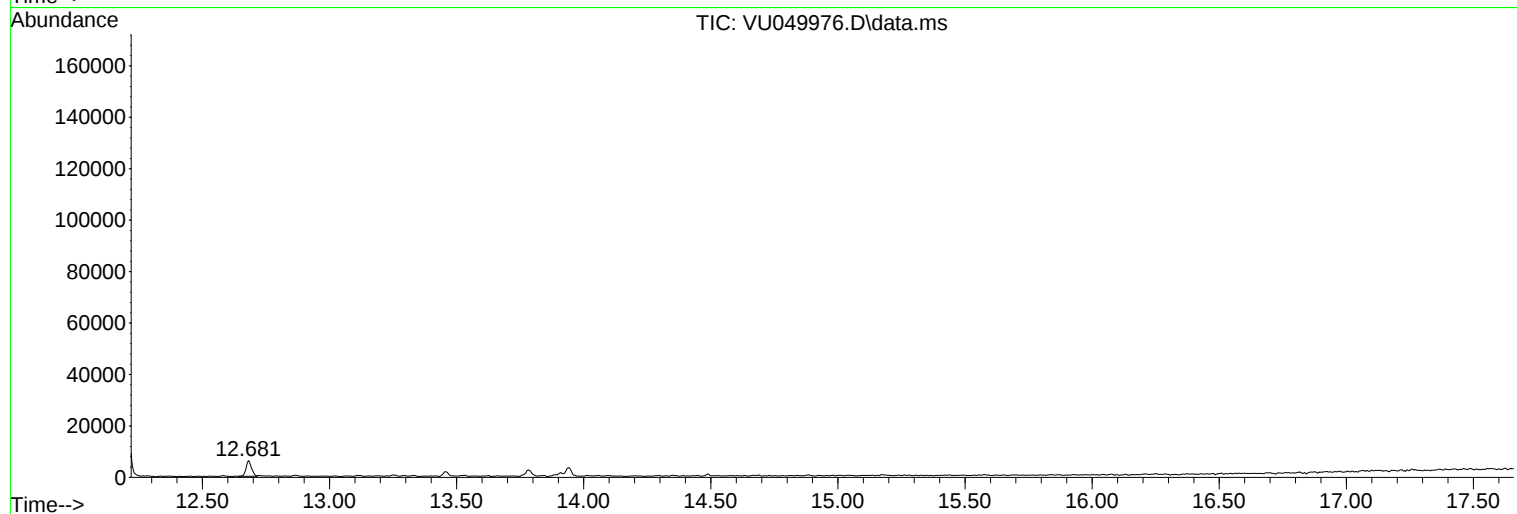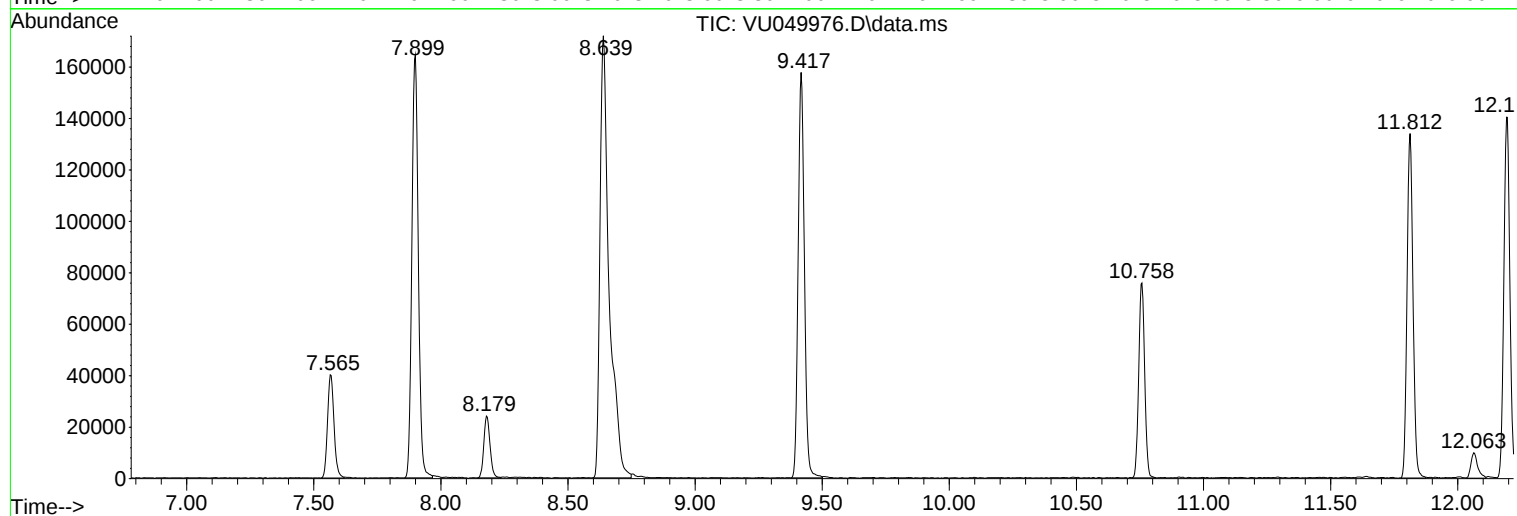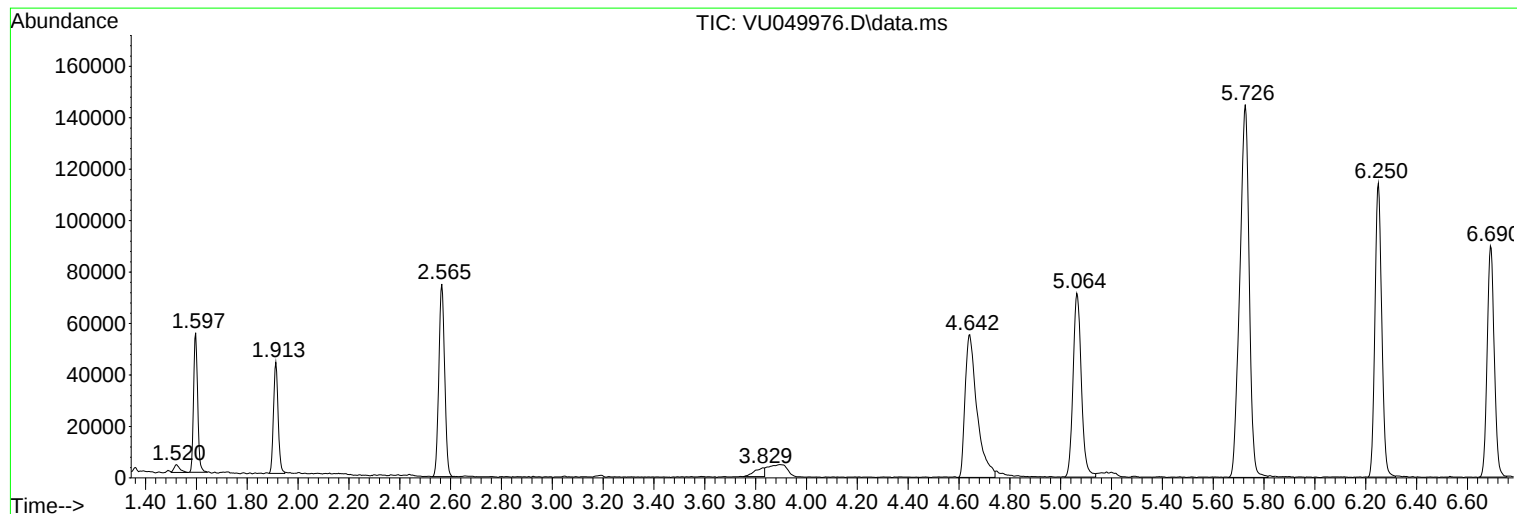

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072722\
Data File : VU049976.D
Acq On : 28 Jul 2022 03:34
Operator : SY/MD
Sample : N3922-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0C90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072722\
Data File : VU049976.D
Acq On : 28 Jul 2022 03:34
Operator : SY/MD
Sample : N3922-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0C90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc