


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072722\
Data File : VU049949.D
Acq On : 27 Jul 2022 14:32
Operator : SY/MD
Sample : BFB095
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB095

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Jul 28 03:41:29 2022

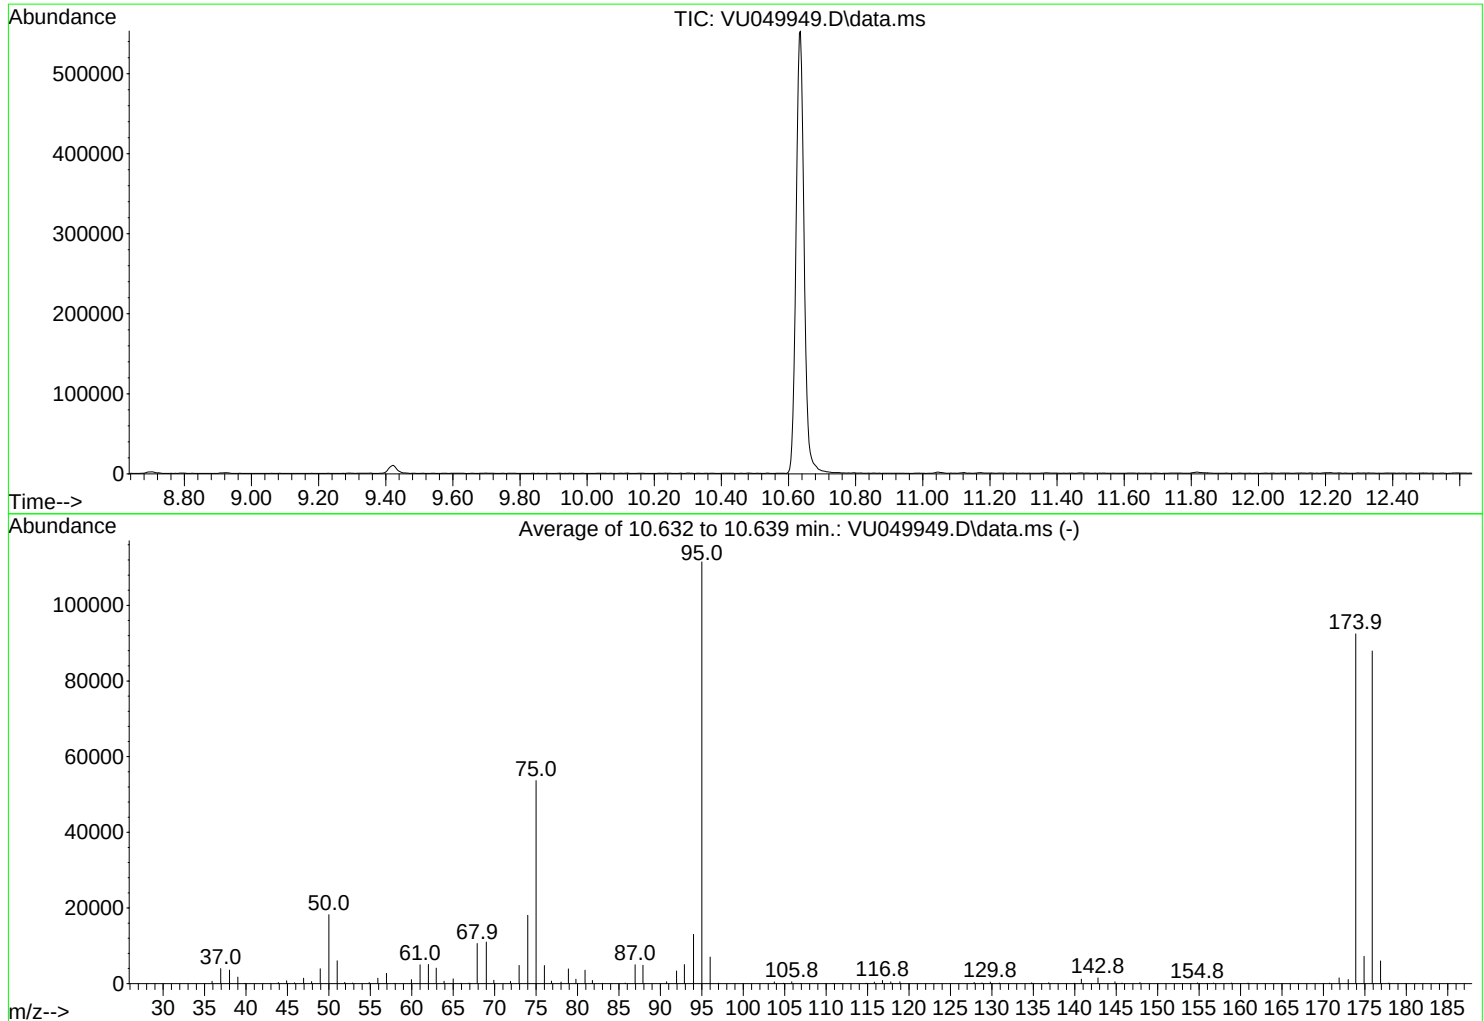

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	18224	PASS
75	95	30	80	48.1	53685	PASS
95	95	100	100	100.0	111499	PASS
96	95	5	9	6.3	7036	PASS
173	174	0.00	2	1.2	1100	PASS
174	95	50	120	82.9	92456	PASS
175	174	5	9	7.8	7227	PASS
176	174	95	101	95.1	87917	PASS
177	176	5	9	6.8	5999	PASS

m/z	Abundance
39.90	185.0
43.90	551.0

Instrument :
MSVOA_U
ClientSampleId :
BFB095

m/z	Abundance
35.90	673.0
36.90	4081.0
38.00	3813.0
39.00	1736.0
39.90	246.0
43.00	123.0
44.00	915.0
44.90	775.0
45.80	247.0
47.00	1521.0
47.90	573.0
49.00	4245.0
50.00	18656.0
51.00	6209.0
51.80	330.0
52.80	203.0
54.80	311.0
55.90	1538.0
57.00	2758.0
58.00	151.0
60.00	1111.0
61.00	5323.0
62.00	5216.0
62.90	4124.0
63.90	620.0
65.00	1223.0
66.00	127.0
66.90	269.0
67.90	11104.0
69.00	11513.0
69.90	981.0
71.90	588.0
72.90	5050.0
74.00	19168.0
75.00	56200.0
76.00	5071.0
76.80	688.0
78.00	438.0
78.90	3930.0
79.80	1251.0
80.90	3603.0
81.80	846.0
83.00	110.0
85.70	165.0
87.00	5346.0
87.90	5417.0
90.80	513.0
91.90	3487.0
92.90	5155.0
94.00	13240.0
95.00	114040.0
96.00	7516.0
97.00	159.0
103.80	482.0
104.90	163.0
105.90	481.0
106.90	159.0
110.90	152.0
114.80	125.0
115.80	489.0
116.80	777.0
117.80	518.0
118.90	561.0
127.80	373.0
128.80	241.0
129.80	358.0
130.90	188.0
134.80	207.0
136.90	289.0
140.00	105.0
140.80	1296.0
142.80	1556.0
144.90	491.0
145.70	217.0
147.90	316.0
154.80	191.0
155.90	128.0
156.70	170.0
158.90	170.0
160.90	171.0
170.70	121.0
171.90	1603.0
173.00	1250.0
173.90	92120.0
174.90	7361.0
175.90	88720.0
176.90	6021.0
177.90	188.0

Instrument :
MSVOA_U
ClientSampleId :
BFB095

m/z	Abundance
35.90	646.0
36.90	3990.0
38.00	3672.0
39.00	1805.0
39.90	268.0
44.00	869.0
44.90	752.0
45.80	233.0
47.00	1474.0
47.90	582.0
49.00	3992.0
50.00	18816.0
51.00	6292.0
51.90	329.0
52.80	193.0
54.80	281.0
55.90	1529.0
57.00	2801.0
57.90	143.0
59.90	1111.0
61.00	5103.0
62.00	5196.0
63.00	4212.0
63.90	650.0
65.00	1335.0
66.00	109.0
66.90	241.0
67.90	10942.0
69.00	11328.0
69.90	948.0
71.90	622.0
73.00	4930.0
74.00	18560.0
75.00	55232.0
76.00	4935.0
76.80	716.0
78.00	466.0
78.90	4022.0
79.80	1223.0
80.90	3605.0
81.80	875.0
83.00	101.0
85.70	169.0
87.00	5126.0
87.90	4909.0
90.80	543.0
91.90	3395.0
92.90	5237.0
94.00	13510.0
95.00	114592.0
96.00	7175.0
97.00	142.0
103.80	475.0
104.90	161.0
105.80	550.0
106.90	122.0
110.80	126.0
112.90	113.0
114.80	128.0
115.80	437.0
116.80	884.0
117.80	508.0
118.90	512.0
127.90	338.0
128.80	239.0
129.80	417.0
130.90	186.0
134.80	252.0
136.80	270.0
140.00	108.0
140.80	1201.0
142.80	1564.0
144.80	482.0
145.70	167.0
147.80	336.0
154.80	225.0
156.00	121.0
156.70	158.0
158.90	186.0
160.90	194.0
170.80	186.0
171.90	1595.0
173.00	1092.0
173.90	95400.0
174.90	7500.0
175.90	90680.0
176.90	6214.0
177.90	191.0

Instrument :
MSVOA_U
ClientSampleId :
BFB095

m/z	Abundance
35.90	597.0
37.00	3847.0
38.00	3319.0
39.00	1699.0
39.80	309.0
42.90	121.0
43.90	796.0
44.90	719.0
45.90	180.0
46.90	1333.0
47.90	519.0
48.90	3518.0
50.00	17200.0
51.00	5695.0
52.00	317.0
52.90	152.0
54.90	276.0
55.90	1317.0
56.90	2590.0
59.90	966.0
61.00	4498.0
62.00	4831.0
63.00	3943.0
63.90	584.0
65.00	1252.0
65.90	100.0
67.10	159.0
67.90	9814.0
69.00	10114.0
69.90	758.0
71.90	563.0
73.00	4439.0
74.00	16432.0
75.00	49624.0
76.00	4299.0
76.90	625.0
78.00	408.0
78.90	3727.0
79.80	1051.0
80.90	3458.0
81.80	828.0
85.80	170.0
86.90	4448.0
87.90	4296.0
90.70	520.0
92.00	3093.0
92.90	4670.0
94.00	12392.0
95.00	105864.0
96.00	6416.0
97.00	147.0
103.70	386.0
104.80	124.0
105.80	545.0
111.70	114.0
112.00	126.0
112.90	124.0
114.80	107.0
115.80	369.0
116.80	864.0
117.80	432.0
118.90	510.0
127.80	326.0
128.80	193.0
129.80	450.0
130.90	168.0
134.80	248.0
136.80	241.0
139.80	112.0
140.80	1122.0
142.80	1475.0
144.80	500.0
145.80	125.0
147.80	296.0
154.80	244.0
156.80	147.0
158.90	142.0
160.90	167.0
170.80	242.0
171.90	1422.0
173.00	959.0
173.90	89848.0
174.90	6821.0
175.90	84352.0
176.90	5762.0
177.90	172.0

Instrument :
MSVOA_U
ClientSampleId :
BFB095