

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072723\
 Data File : VU054891.D
 Acq On : 27 Jul 2023 11:14
 Operator : MD/SY
 Sample : VU0727WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0727WBL01

Quant Time: Jul 28 05:43:05 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Wed Jul 26 09:45:35 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.110	96	24523	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.634	95	7466	1.004	ug/l	0.00
Spiked Amount 1.000			Recovery	=	100.000%	
68) 1,2-Dichlorobenzene-d4	12.193	152	8202	0.976	ug/l	0.00
Spiked Amount 1.000			Recovery	=	98.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072723\
Data File : VU054891.D
Acq On : 27 Jul 2023 11:14
Operator : MD/SY
Sample : VU0727WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0727WBL01

Quant Time: Jul 28 05:43:05 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Wed Jul 26 09:45:35 2023
Response via : Initial Calibration




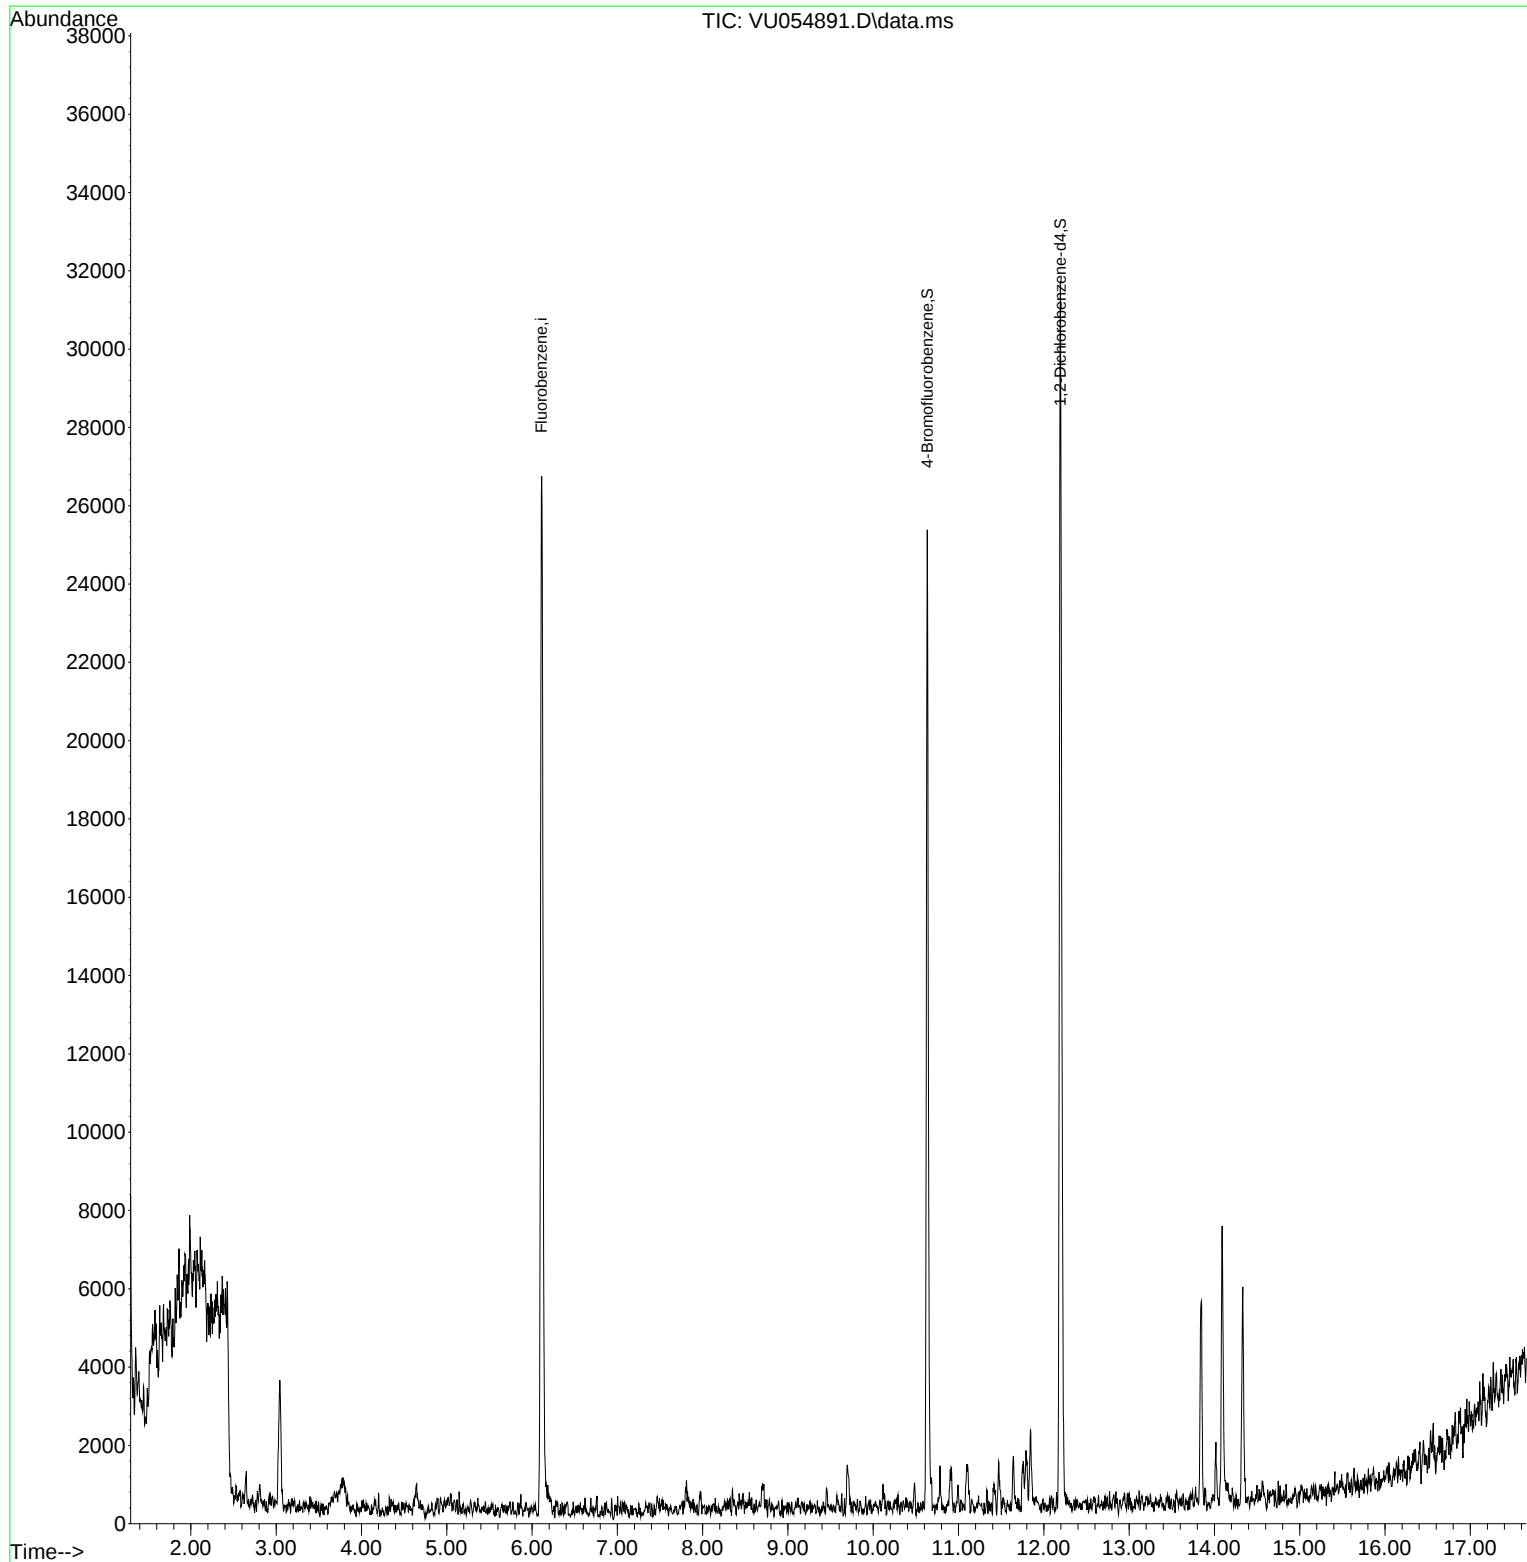


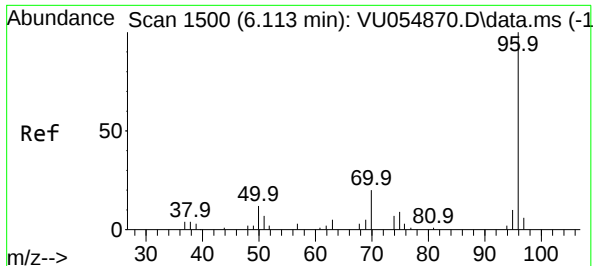

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.110 min Scan# 1499
Delta R.T. -0.003 min
Lab File: VU054891.D
Acq: 27 Jul 2023 11:14




Instrument :
MSVOA_U
ClientSampleId :
VU0727WBL01


Tgt Ion: 96	Resp: 24523
Ion Ratio	Lower Upper
96 100	
70 17.8	14.0 21.0
95 10.0	8.7 13.1
97 7.2	0.0 0.0

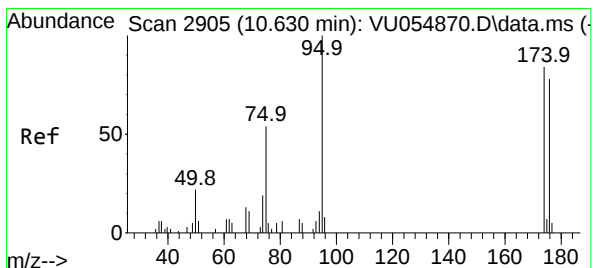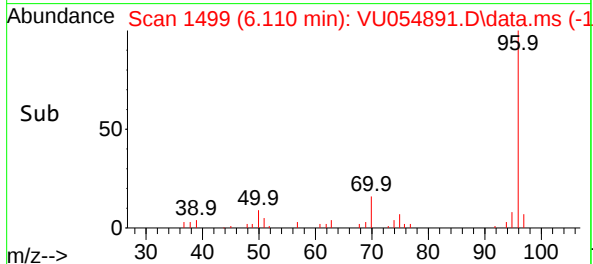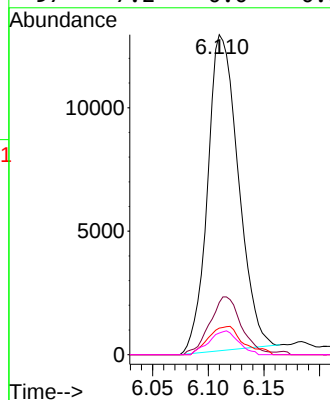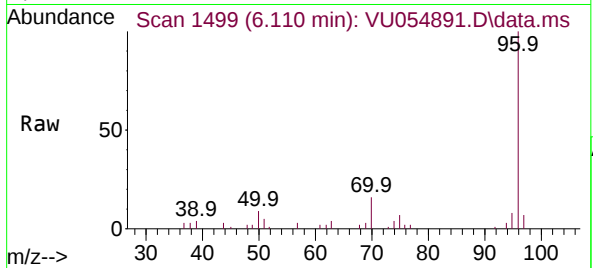

#57
4-Bromofluorobenzene
Concen: 1.004 ug/l
RT: 10.634 min Scan# 2906
Delta R.T. 0.003 min
Lab File: VU054891.D
Acq: 27 Jul 2023 11:14


Tgt Ion: 95	Resp: 7466
Ion Ratio	Lower Upper
95 100	
174 93.7	79.3 118.9
176 95.4	71.5 107.3

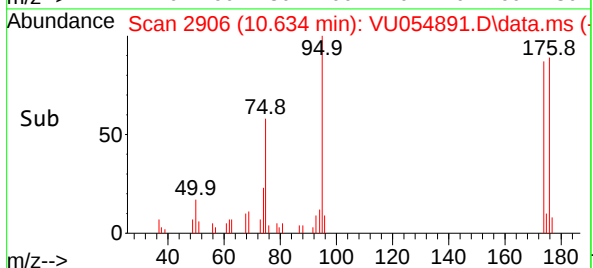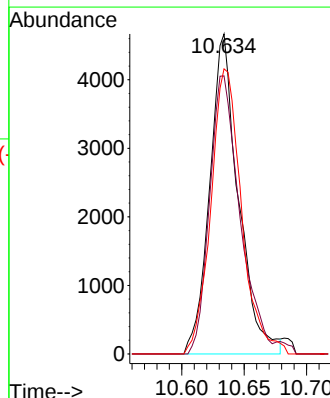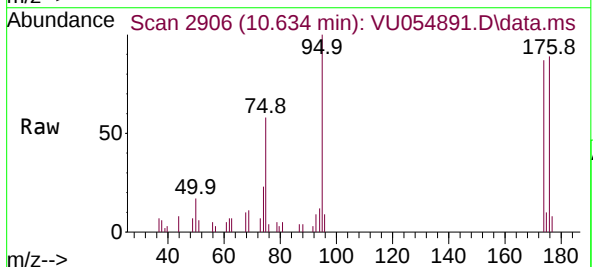

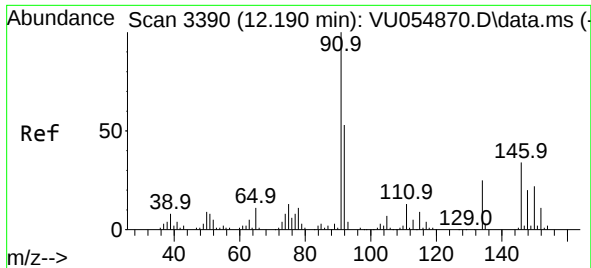

#68
1,2-Dichlorobenzene-d4
Concen: 0.976 ug/l
RT: 12.193 min Scan# 31
Delta R.T. 0.003 min
Lab File: VU054891.D
Acq: 27 Jul 2023 11:14

Instrument :
MSVOA_U
ClientSampleId :
VU0727WBL01

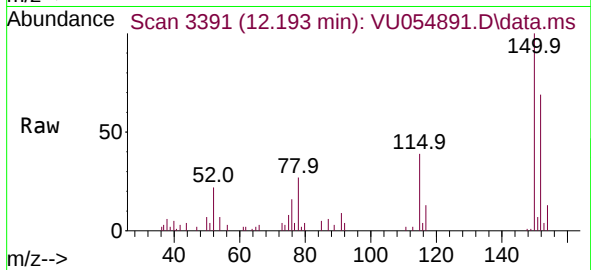

Tgt Ion:	152	Resp:	8202
Ion	Ratio	Lower	Upper
152	100		
115	58.3	0.0	234.8
150	155.0	0.0	598.2

