

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072723\
 Data File : VU054897.D
 Acq On : 27 Jul 2023 16:28
 Operator : MD/SY
 Sample : VIBLK
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Quant Time: Jul 28 05:46:04 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Wed Jul 26 09:45:35 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Fluorobenzene	6.116	96	25566	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.637	95	7595	0.980	ug/l	0.00
Spiked Amount 1.000			Recovery	=	98.000%	
68) 1,2-Dichlorobenzene-d4	12.196	152	8198	0.936	ug/l	0.00
Spiked Amount 1.000			Recovery	=	94.000%	
Target Compounds						
15) Methylene Chloride	3.043	84	10001	1.733	ug/l	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072723\
Data File : VU054897.D
Acq On : 27 Jul 2023 16:28
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Time: Jul 28 05:46:04 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Wed Jul 26 09:45:35 2023
Response via : Initial Calibration




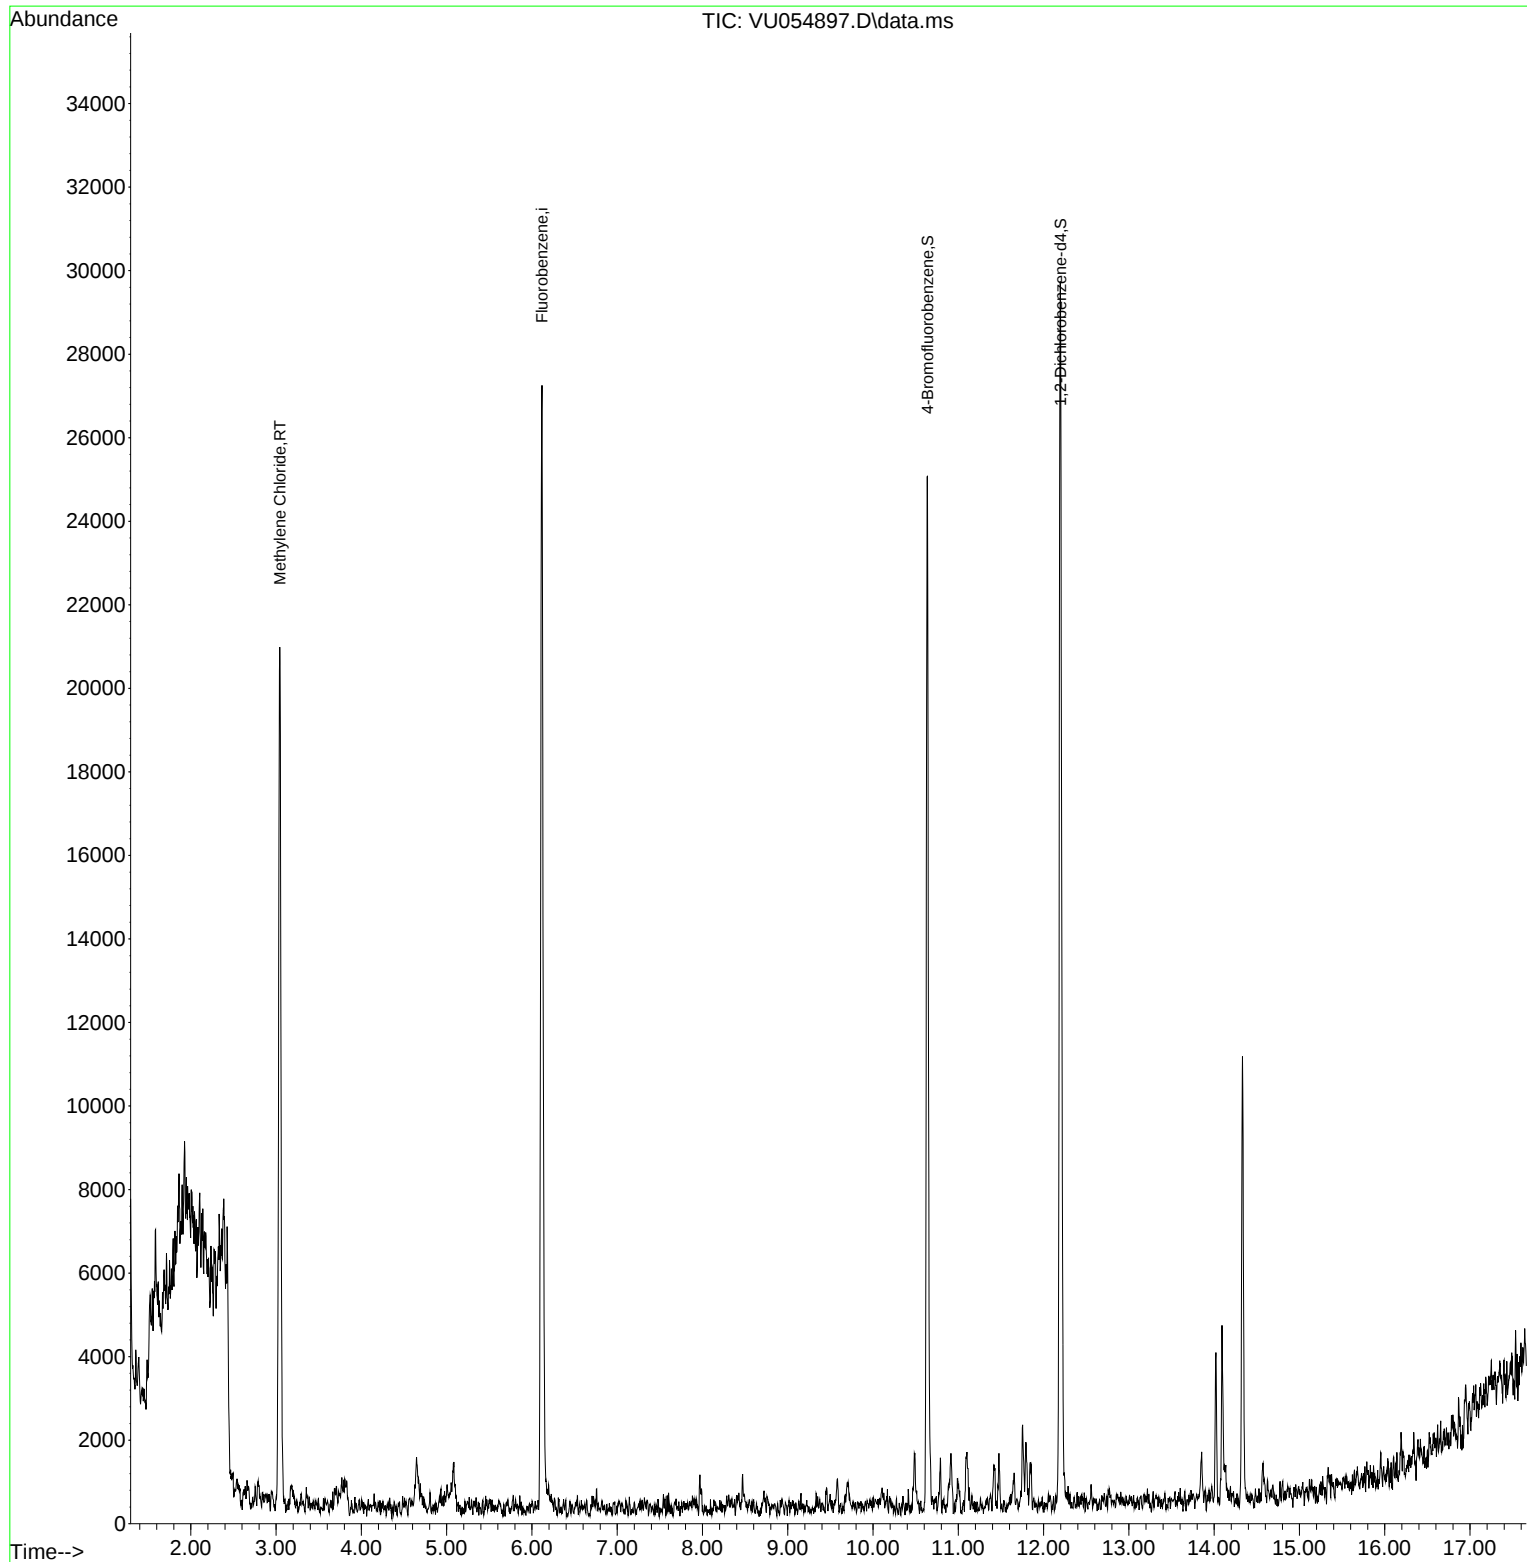


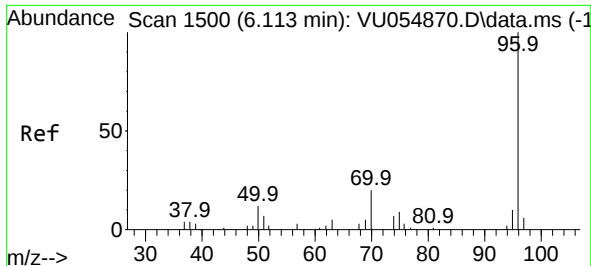

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.116 min Scan# 1501
Delta R.T. 0.003 min
Lab File: VU054897.D
Acq: 27 Jul 2023 16:28




Instrument :
MSVOA_U
ClientSampleId :
VIBLK


Tgt Ion:	96	Resp:	25566
Ion	Ratio	Lower	Upper
96	100		
70	18.5	14.0	21.0
95	9.3	8.7	13.1
97	6.2	0.0	0.0

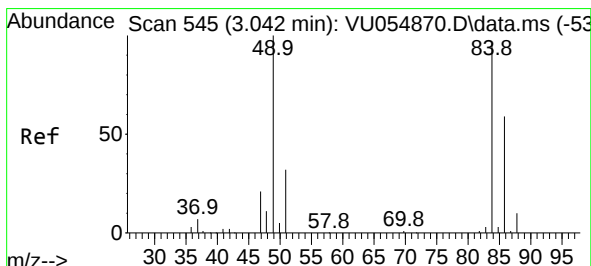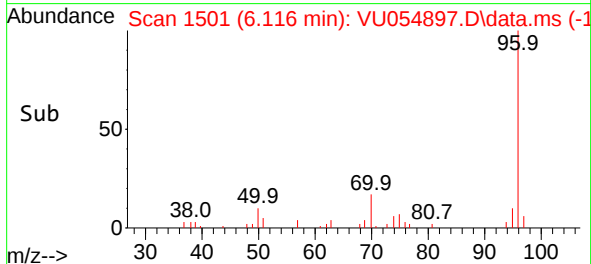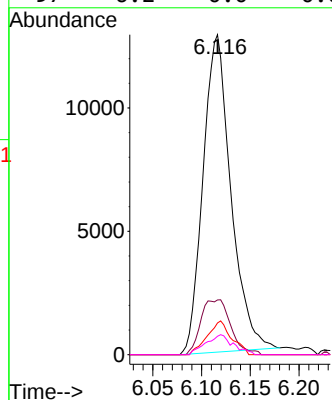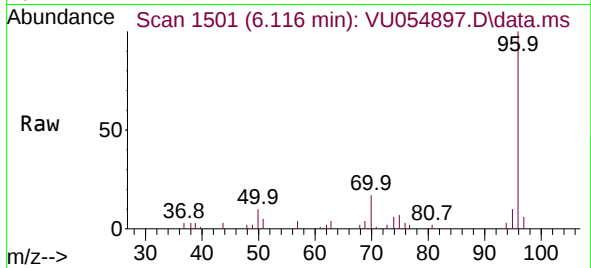

#15
Methylene Chloride
Concen: 1.733 ug/l
RT: 3.043 min Scan# 545
Delta R.T. 0.000 min
Lab File: VU054897.D
Acq: 27 Jul 2023 16:28

Tgt Ion:	84	Resp:	10001
Ion	Ratio	Lower	Upper
84	100		
49	111.7	87.8	131.6
51	39.4	0.0	68.2
86	69.9	51.0	76.4

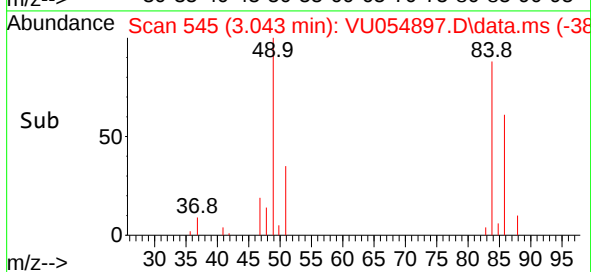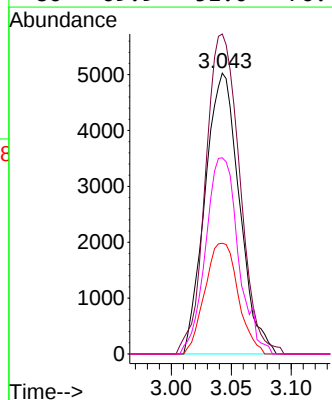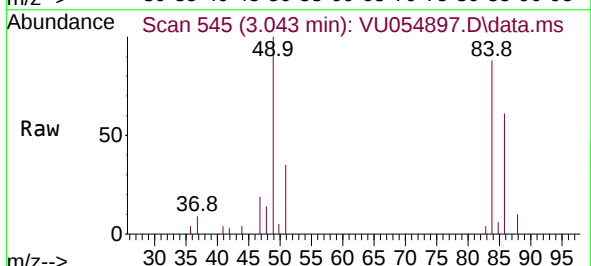

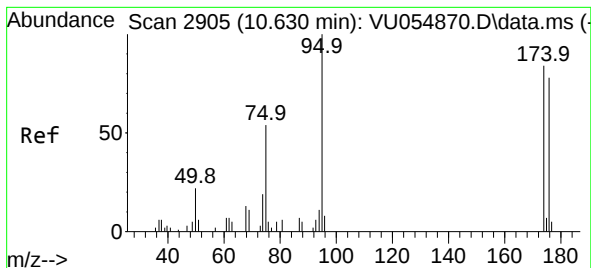

#57

4-Bromofluorobenzene

Concen: 0.980 ug/l

RT: 10.637 min Scan# 2905

Delta R.T. 0.007 min

Lab File: VU054897.D

Acq: 27 Jul 2023 16:28

Instrument :

MSVOA_U

ClientSampleId :

VIBLK





Tgt Ion: 95 Resp: 7595

Ion Ratio Lower Upper

95 100

174 96.2 79.3 118.9

176 93.8 71.5 107.3

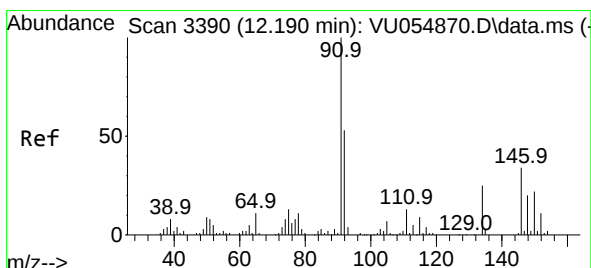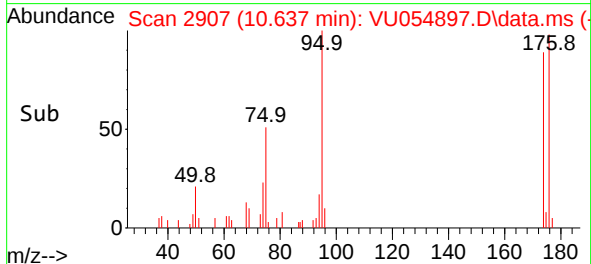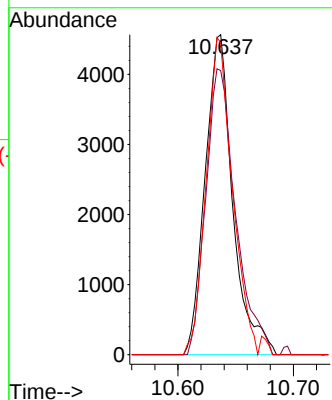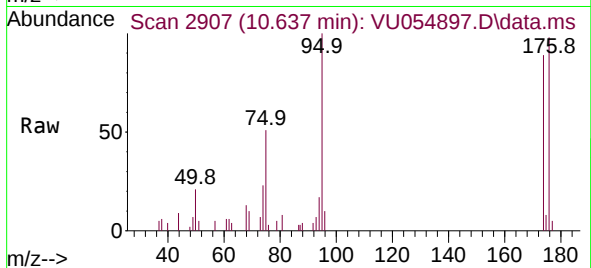

#68

1,2-Dichlorobenzene-d4

Concen: 0.936 ug/l

RT: 12.196 min Scan# 3392

Delta R.T. 0.007 min

Lab File: VU054897.D

Acq: 27 Jul 2023 16:28

Tgt Ion:152 Resp: 8198

Ion Ratio Lower Upper

152 100

115 61.4 0.0 234.8

150 161.6 0.0 598.2

