

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072723\
 Data File : VU054891.D
 Acq On : 27 Jul 2023 11:14
 Operator : MD/SY
 Sample : VU0727WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0727WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU054891.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.817	161	164	167	rBV3	1436	1035	1.75%	0.439%
2	1.985	214	216	226	rVB10	2085	2201	3.71%	0.933%
3	2.071	241	243	246	rBV3	1092	710	1.20%	0.301%
4	2.110	253	255	259	rBV5	1340	805	1.36%	0.341%
5	2.425	351	353	363	rVB5	4987	5891	9.94%	2.496%
6	2.650	415	423	428	rVV3	841	928	1.57%	0.393%
7	3.042	535	545	553	rBV6	3150	5900	9.96%	2.500%
8	4.647	1035	1044	1046	rVV2	587	787	1.33%	0.334%
9	6.113	1488	1500	1515	rBV2	26533	53192	89.76%	22.542%
10	7.467	1915	1921	1927	rBV	465	660	1.11%	0.280%
11	8.351	2192	2196	2201	rBV3	675	694	1.17%	0.294%
12	8.473	2228	2234	2239	rVB2	523	645	1.09%	0.273%
13	9.454	2535	2539	2543	rBV2	648	738	1.25%	0.313%
14	9.695	2607	2614	2619	rBV3	1259	1881	3.17%	0.797%
15	10.116	2737	2745	2748	rBV3	690	738	1.25%	0.313%
16	10.483	2851	2859	2865	rVB2	837	1101	1.86%	0.467%
17	10.634	2895	2906	2918	rBV3	25011	39866	67.27%	16.894%
18	10.782	2949	2952	2959	rVB3	1116	935	1.58%	0.396%
19	10.904	2984	2990	2991	rBV2	950	813	1.37%	0.345%
20	10.914	2991	2993	3000	rVB2	1110	1039	1.75%	0.440%
21	10.994	3014	3018	3025	rVB3	699	738	1.25%	0.313%
22	11.097	3043	3050	3051	rBV2	1180	1216	2.05%	0.515%
23	11.106	3051	3053	3058	rVB2	832	704	1.19%	0.298%
24	11.470	3159	3166	3172	rBV2	1354	1923	3.24%	0.815%
25	11.643	3211	3220	3225	rBV4	1404	1895	3.20%	0.803%
26	11.750	3248	3253	3255	rBV4	1144	1188	2.00%	0.503%
27	11.791	3260	3266	3268	rBV5	973	830	1.40%	0.352%
28	11.843	3275	3282	3290	rVB6	1830	2580	4.35%	1.093%
29	12.193	3381	3391	3407	rBV5	31340	59261	100.00%	25.114%
30	13.557	3809	3815	3818	rBV4	557	697	1.18%	0.295%
31	13.846	3895	3905	3915	rVB5	5211	8320	14.04%	3.526%
32	14.016	3953	3958	3964	rBV5	1482	1521	2.57%	0.645%
33	14.090	3969	3981	3995	rBV	7143	11927	20.13%	5.054%
34	14.331	4045	4056	4064	rBV7	5571	8551	14.43%	3.624%
35	16.409	4700	4702	4706	rVB2	1073	686	1.16%	0.291%
36	16.450	4706	4715	4718	rBV6	1118	1581	2.67%	0.670%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072723\
Data File : VU054891.D
Acq On : 27 Jul 2023 11:14
Operator : MD/SY
Sample : VU0727WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0727WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

37	16.534	4737	4741	4744	rVV3	1011	906	1.53%	0.384%
38	16.566	4747	4751	4754	rVV	1270	1124	1.90%	0.476%
39	16.675	4782	4785	4790	rVB2	802	640	1.08%	0.271%
40	16.727	4797	4801	4808	rBV7	751	885	1.49%	0.375%
41	16.865	4841	4844	4848	rBV3	827	760	1.28%	0.322%
42	16.939	4864	4867	4871	rVV3	878	806	1.36%	0.342%
43	16.987	4879	4882	4887	rBV4	777	635	1.07%	0.269%
44	17.109	4918	4920	4926	rVB6	1113	925	1.56%	0.392%
45	17.148	4928	4932	4934	rBV5	1139	827	1.40%	0.350%
46	17.216	4946	4953	4957	rBV7	972	1326	2.24%	0.562%
47	17.238	4958	4960	4965	rVV6	945	697	1.18%	0.295%
48	17.270	4967	4970	4974	rVV5	1133	871	1.47%	0.369%
49	17.306	4977	4981	4985	rVV4	633	653	1.10%	0.277%
50	17.540	5050	5054	5057	rVB4	906	740	1.25%	0.314%




Sum of corrected areas: 235972

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072723\
Data File : VU054891.D
Acq On : 27 Jul 2023 11:14
Operator : MD/SY
Sample : VU0727WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0727WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

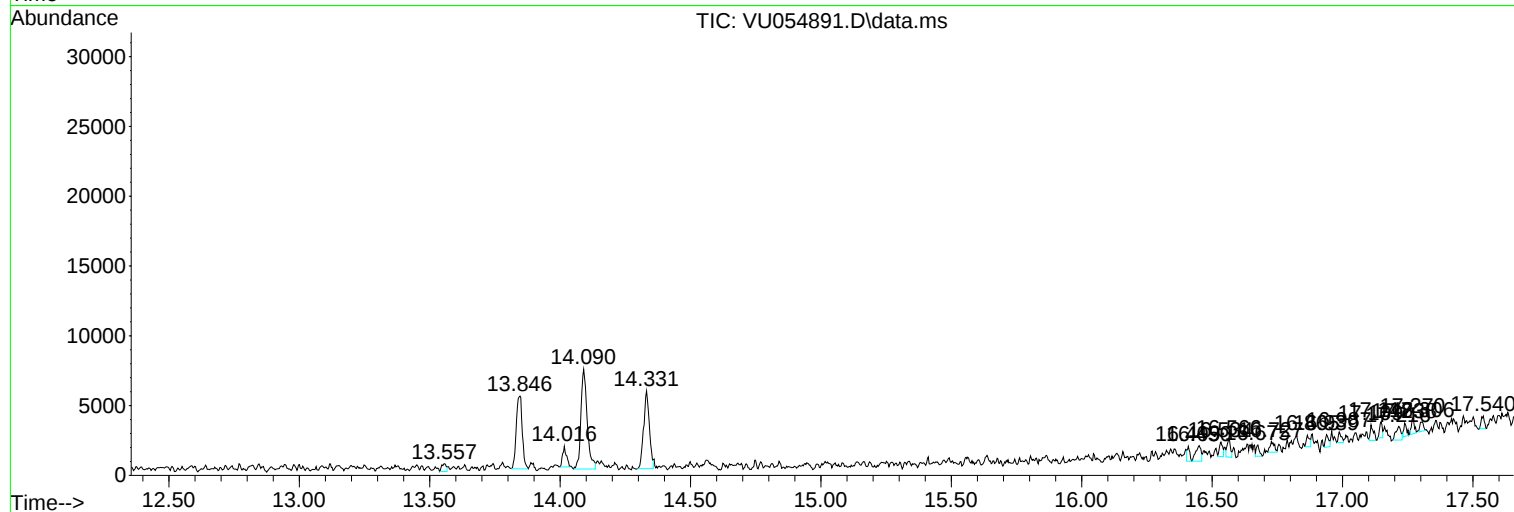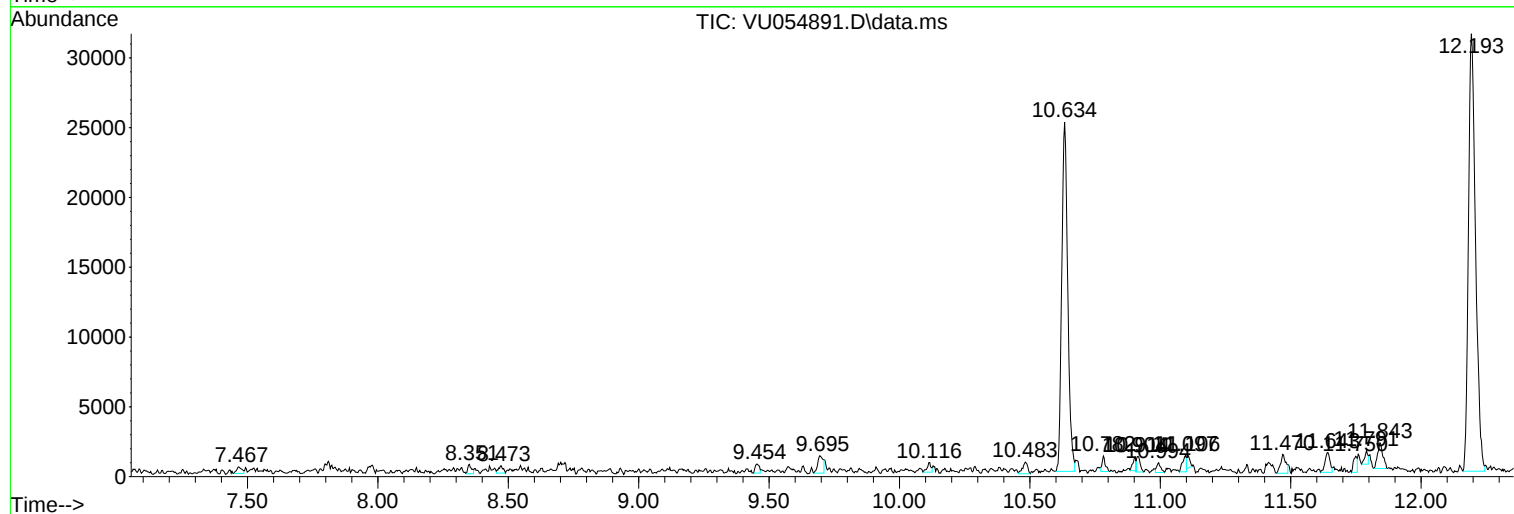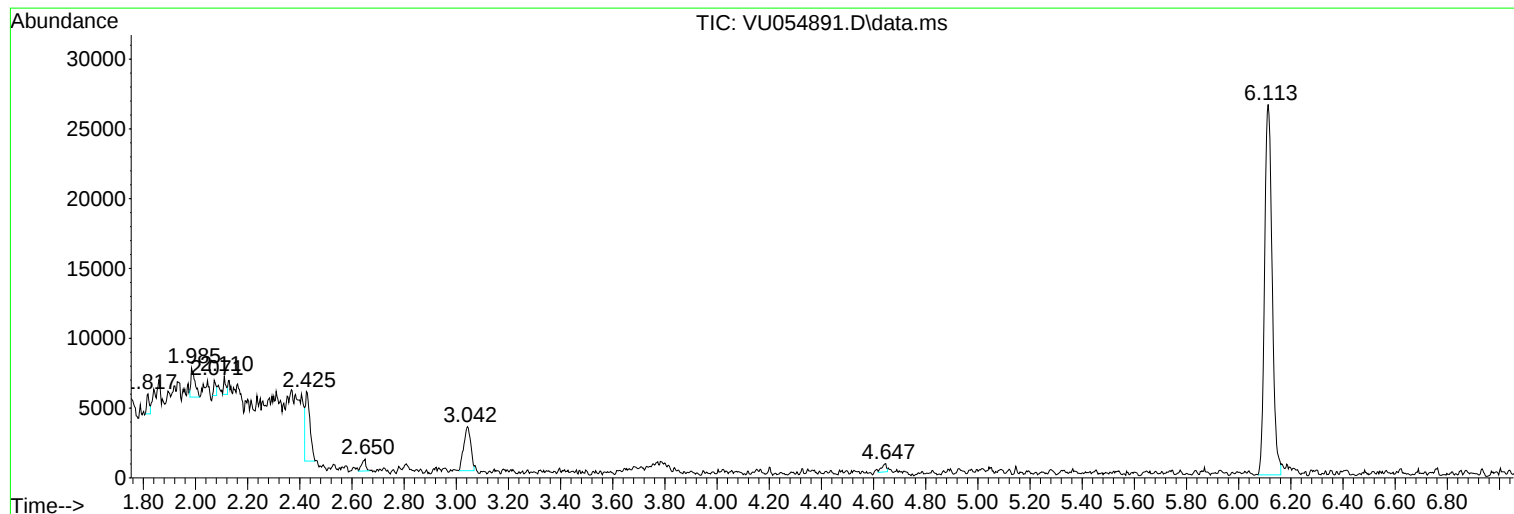

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072723\
Data File : VU054891.D
Acq On : 27 Jul 2023 11:14
Operator : MD/SY
Sample : VU0727WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0727WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072723\
Data File : VU054891.D
Acq On : 27 Jul 2023 11:14
Operator : MD/SY
Sample : VU0727WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0727WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------