

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072723\
 Data File : VU054897.D
 Acq On : 27 Jul 2023 16:28
 Operator : MD/SY
 Sample : VIBLK
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU054897.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.235	292	294	297	rBV3	1294	756	1.34%	0.293%
2	2.271	303	305	307	rBV3	1600	994	1.76%	0.385%
3	2.425	351	353	365	rVB2	5928	6717	11.87%	2.602%
4	3.043	528	545	561	rBV2	20685	40561	71.65%	15.711%
5	4.567	1012	1019	1023	rBV2	415	647	1.14%	0.251%
6	4.647	1039	1044	1050	rVV2	823	1127	1.99%	0.437%
7	5.084	1172	1180	1183	rBV4	716	798	1.41%	0.309%
8	6.116	1489	1501	1515	rBV2	26928	52399	92.56%	20.297%
9	7.968	2072	2077	2082	rBV2	977	1151	2.03%	0.446%
10	8.470	2226	2233	2236	rBV3	859	784	1.38%	0.304%
11	9.582	2573	2579	2584	rVB3	793	1038	1.83%	0.402%
12	10.489	2855	2861	2867	rVB2	1057	1332	2.35%	0.516%
13	10.637	2894	2907	2923	rBV2	24751	41538	73.38%	16.090%
14	10.788	2950	2954	2960	rVB2	1326	1264	2.23%	0.490%
15	10.914	2985	2993	3001	rVB4	1452	2654	4.69%	1.028%
16	11.090	3042	3048	3049	rBV	1325	1166	2.06%	0.452%
17	11.415	3142	3149	3152	rBV2	1114	1398	2.47%	0.542%
18	11.476	3161	3168	3175	rVB2	1327	1618	2.86%	0.627%
19	11.753	3249	3254	3261	rBV4	1729	2119	3.74%	0.821%
20	11.791	3261	3266	3273	rVB3	1268	1562	2.76%	0.605%
21	11.843	3276	3282	3283	rBV4	1032	873	1.54%	0.338%
22	12.193	3378	3391	3405	rVV3	29241	56608	100.00%	21.927%
23	12.557	3498	3504	3509	rVB	583	604	1.07%	0.234%
24	13.852	3899	3907	3914	rVB3	1221	1753	3.10%	0.679%
25	14.020	3950	3959	3966	rVB7	3586	4362	7.71%	1.690%
26	14.090	3977	3981	3989	rVV3	3875	4498	7.95%	1.742%
27	14.331	4044	4056	4070	rBV4	10807	16853	29.77%	6.528%
28	14.573	4125	4131	4134	rBV3	912	1162	2.05%	0.450%
29	15.788	4505	4509	4512	rBV3	726	675	1.19%	0.261%
30	15.952	4555	4560	4567	rVB4	835	921	1.63%	0.357%
31	16.103	4603	4607	4610	rBV2	792	768	1.36%	0.297%
32	16.190	4629	4634	4639	rBV6	998	983	1.74%	0.381%
33	16.389	4689	4696	4698	rBV4	987	1159	2.05%	0.449%
34	16.865	4841	4844	4848	rBV4	1143	928	1.64%	0.359%
35	16.933	4862	4865	4867	rBV2	925	628	1.11%	0.243%
36	16.991	4878	4883	4889	rBV6	786	1016	1.79%	0.394%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072723\
Data File : VU054897.D
Acq On : 27 Jul 2023 16:28
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER

37	17.399	5005	5010	5012	rBV4	1037	944	1.67%	0.366%
38	17.534	5049	5052	5056	rBV6	1648	1198	2.12%	0.464%
39	17.569	5060	5063	5065	rBV2	925	611	1.08%	0.237%




Sum of corrected areas: 258167

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072723\
Data File : VU054897.D
Acq On : 27 Jul 2023 16:28
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

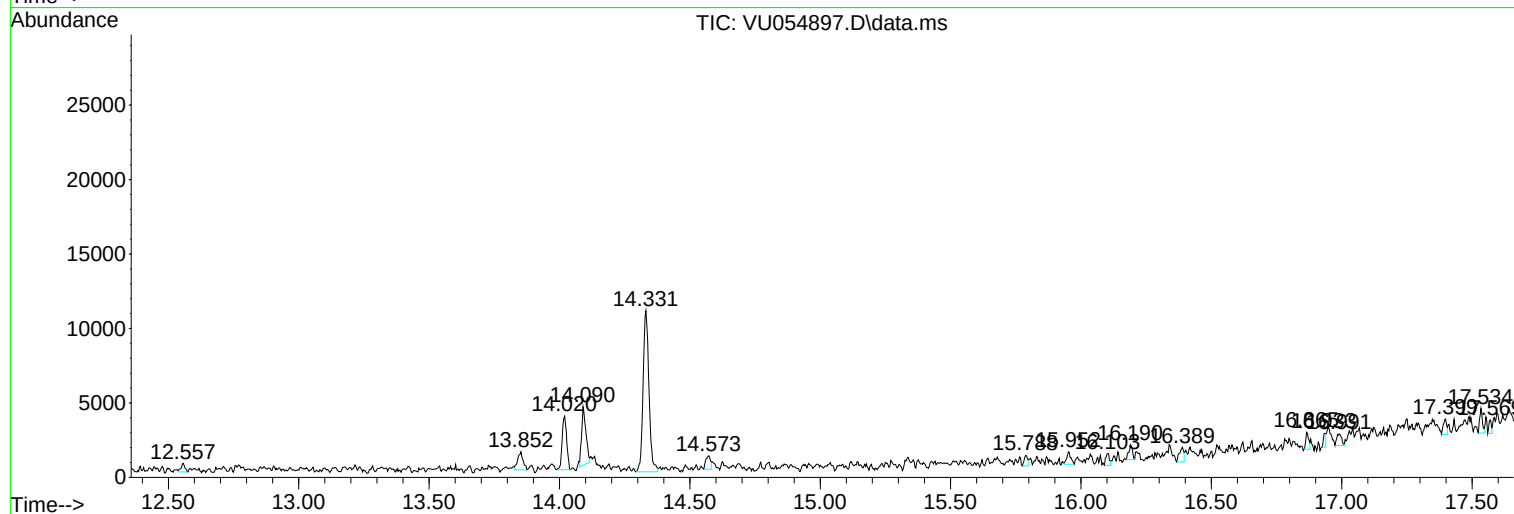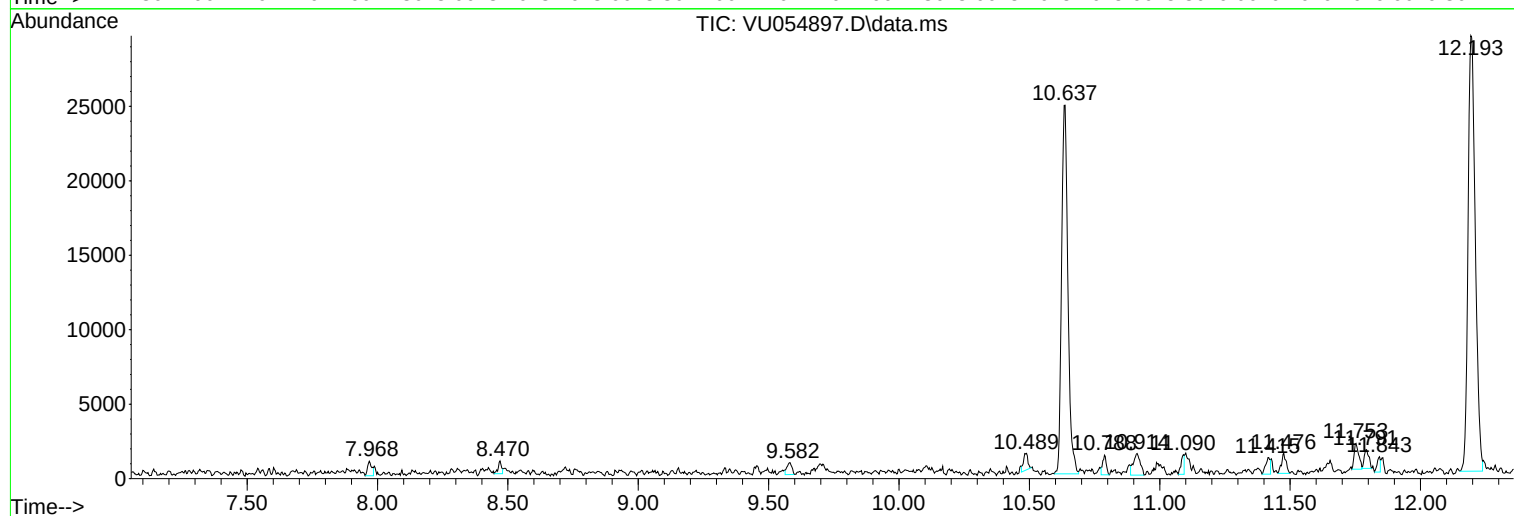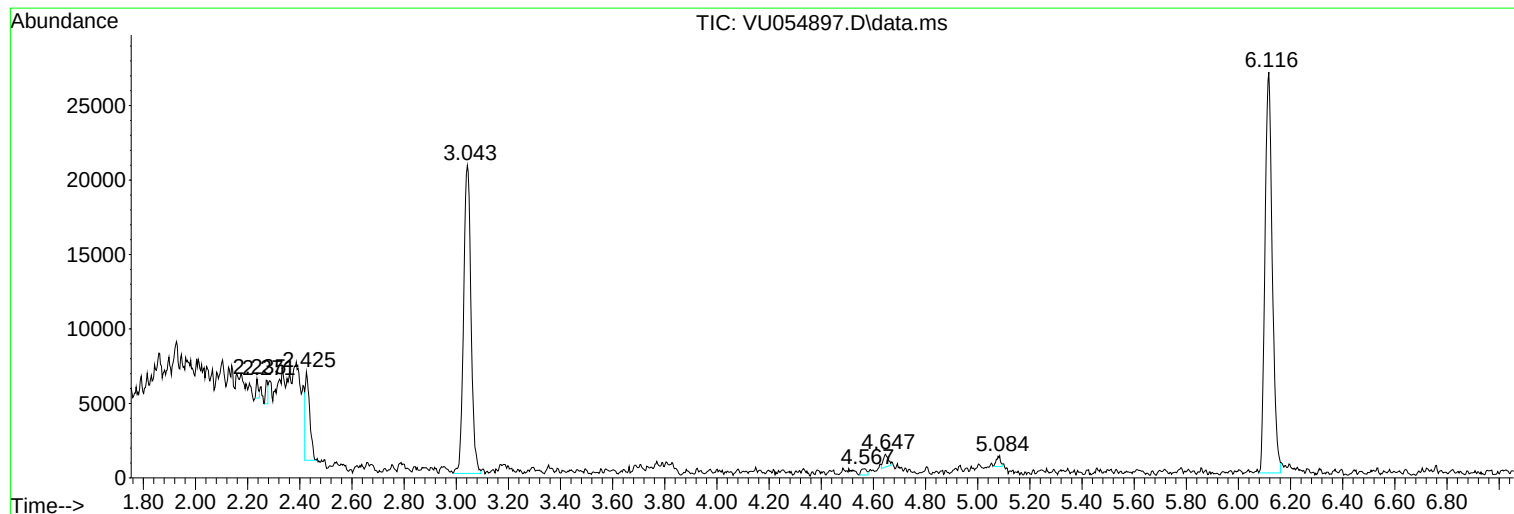

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072723\
Data File : VU054897.D
Acq On : 27 Jul 2023 16:28
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072723\
Data File : VU054897.D
Acq On : 27 Jul 2023 16:28
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------