


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072723\
Data File : VU054889.D
Acq On : 27 Jul 2023 08:45
Operator : MD/SY
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U072523DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Wed Jul 26 09:45:35 2023

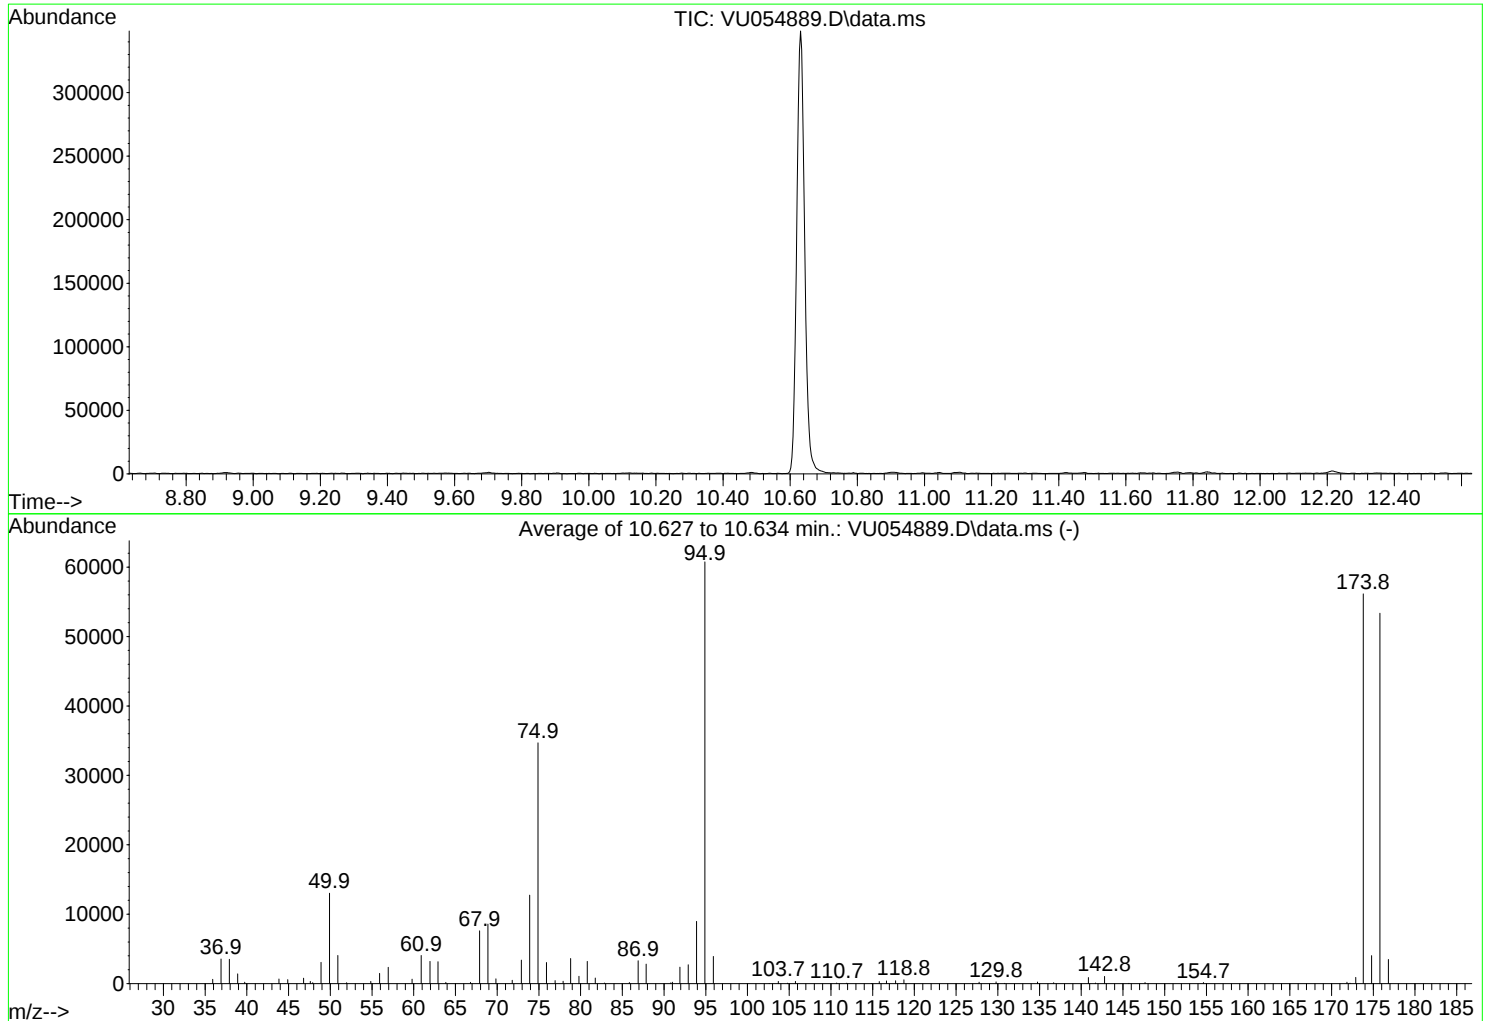

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.4	13015	PASS
75	95	30	60	57.1	34701	PASS
95	95	100	100	100.0	60760	PASS
96	95	5	9	6.5	3930	PASS
173	174	0.00	2	1.6	899	PASS
174	95	50	100	92.4	56136	PASS
175	174	5	9	7.2	4042	PASS
176	174	95	101	95.1	53360	PASS
177	176	5	9	6.5	3492	PASS