

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072822\
 Data File : VU049984.D
 Acq On : 28 Jul 2022 14:16
 Operator : SY/MD
 Sample : N3922-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0C54

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU049984.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.385	7	14	36	rVB	74049	84224	5.85%	1.204%
2	1.601	72	81	102	rBV2	212212	255807	17.78%	3.658%
3	1.909	169	177	192	rBV	38642	49380	3.43%	0.706%
4	2.572	369	383	402	rVB4	121421	234507	16.30%	3.353%
5	3.353	611	626	649	rVB	37180	75910	5.28%	1.085%
6	3.871	773	787	802	rBV	18970	45703	3.18%	0.653%
7	4.662	1010	1033	1069	rBV3	168019	505035	35.10%	7.221%
8	5.083	1143	1164	1185	rBV3	126784	384896	26.75%	5.503%
9	5.318	1222	1237	1253	rVB2	32274	74114	5.15%	1.060%
10	5.726	1342	1364	1386	rBV2	137740	351702	24.44%	5.029%
11	6.250	1511	1527	1550	rBV	116986	222012	15.43%	3.174%
12	6.543	1605	1618	1640	rVB	69823	129411	8.99%	1.850%
13	6.690	1651	1664	1682	rBV	87028	167832	11.66%	2.400%
14	6.790	1682	1695	1715	rVV	168504	315562	21.93%	4.512%
15	7.105	1781	1793	1807	rBV	52107	95524	6.64%	1.366%
16	7.565	1924	1936	1954	rBV	41049	72988	5.07%	1.044%
17	7.899	2024	2040	2056	rBV	153654	264605	18.39%	3.783%
18	8.182	2117	2128	2143	rBV2	24276	41444	2.88%	0.593%
19	8.552	2232	2243	2258	rBV2	109689	181849	12.64%	2.600%
20	8.639	2258	2270	2306	rBV3	173575	414943	28.84%	5.933%
21	8.809	2311	2323	2346	rVV	141325	243472	16.92%	3.481%
22	8.925	2346	2359	2384	rVB	54052	94966	6.60%	1.358%
23	9.446	2500	2521	2554	rBV2	700139	1438901	100.00%	20.574%
24	10.292	2772	2784	2806	rBV	136255	230230	16.00%	3.292%
25	10.758	2917	2929	2945	rBV	72272	117327	8.15%	1.678%
26	11.835	3245	3264	3282	rBV2	256809	612856	42.59%	8.763%
27	12.192	3364	3375	3394	rBV	134679	221035	15.36%	3.160%
28	12.996	3614	3625	3637	rVB	41903	67638	4.70%	0.967%


Sum of corrected areas: 6993873

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072822\
Data File : VU049984.D
Acq On : 28 Jul 2022 14:16
Operator : SY/MD
Sample : N3922-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0C54

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

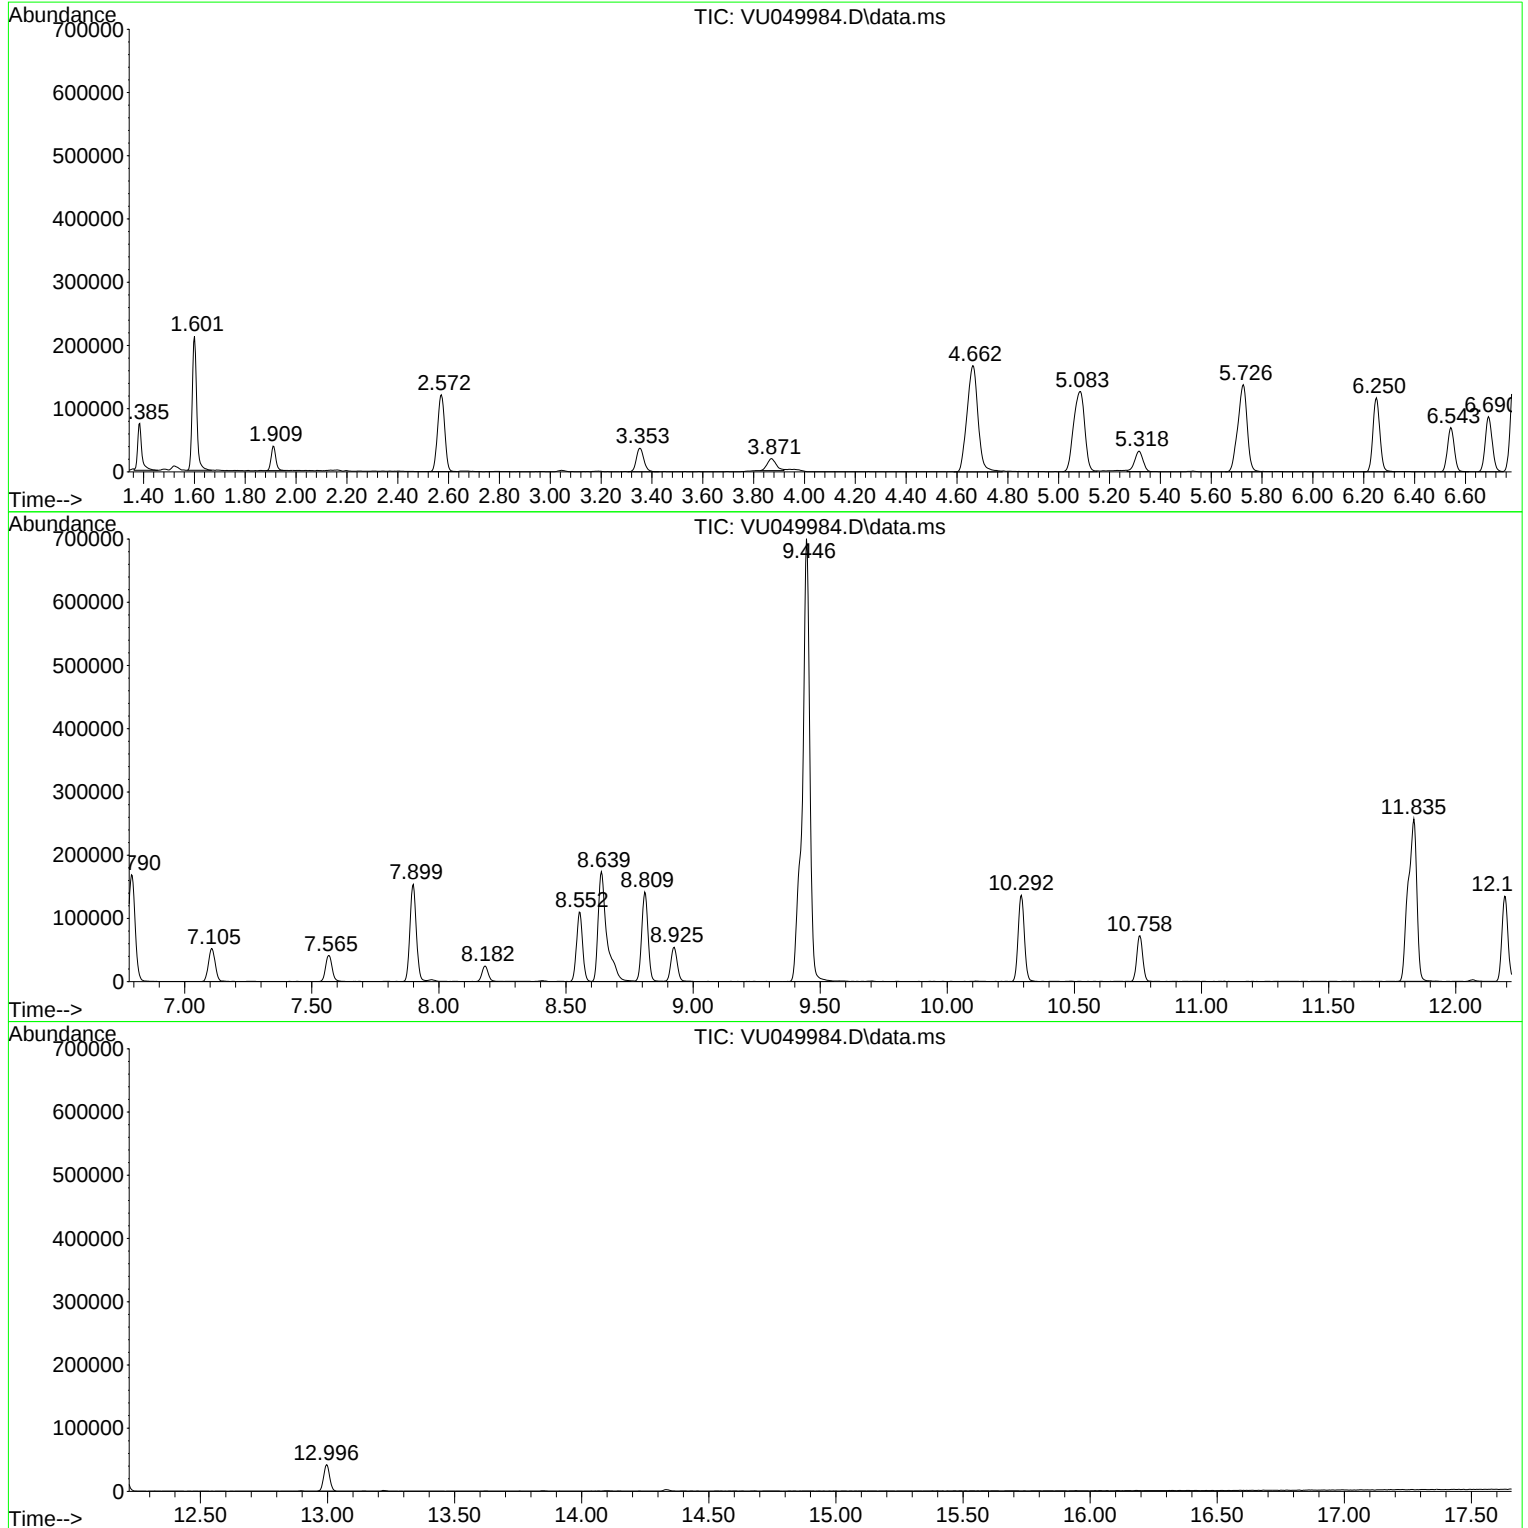

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072822\
Data File : VU049984.D
Acq On : 28 Jul 2022 14:16
Operator : SY/MD
Sample : N3922-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0C54

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072822\
Data File : VU049984.D
Acq On : 28 Jul 2022 14:16
Operator : SY/MD
Sample : N3922-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0C54

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc