

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072822\
 Data File : VU050011.D
 Acq On : 29 Jul 2022 02:13
 Operator : SY/MD
 Sample : N3879-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUH6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU050011.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.359	3	6	11	rVB2	5989	4564	1.14%	0.152%
2	1.597	72	80	97	rVV	44457	50559	12.68%	1.681%
3	1.912	170	178	191	rVB	35089	44778	11.23%	1.489%
4	2.138	239	248	263	rVB	11897	17704	4.44%	0.589%
5	2.565	369	381	394	rVB	58109	92448	23.18%	3.074%
6	3.855	749	782	787	rBV3	5693	22298	5.59%	0.741%
7	4.636	1012	1025	1062	rBV	51567	153686	38.54%	5.110%
8	5.063	1141	1158	1178	rBV2	60002	139721	35.04%	4.645%
9	5.726	1344	1364	1385	rBV2	117146	303421	76.09%	10.088%
10	6.250	1512	1527	1548	rBV	98128	187321	46.98%	6.228%
11	6.543	1608	1618	1631	rVB	20668	36769	9.22%	1.223%
12	6.690	1651	1664	1686	rBV	74708	146762	36.81%	4.880%
13	7.568	1925	1937	1956	rBV2	30969	54755	13.73%	1.821%
14	7.899	2027	2040	2056	rBV	126610	219011	54.93%	7.282%
15	8.182	2118	2128	2144	rBV2	18651	31954	8.01%	1.062%
16	8.552	2231	2243	2258	rBV	233688	398745	100.00%	13.258%
17	8.639	2258	2270	2303	rVB4	148963	368883	92.51%	12.265%
18	9.417	2498	2512	2531	rBV	141089	240191	60.24%	7.986%
19	10.758	2917	2929	2952	rBV	74151	130257	32.67%	4.331%
20	11.812	3238	3257	3272	rBV	116060	187000	46.90%	6.217%
21	12.195	3364	3376	3393	rBV	109500	176857	44.35%	5.880%




Sum of corrected areas: 3007684

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072822\
Data File : VU050011.D
Acq On : 29 Jul 2022 02:13
Operator : SY/MD
Sample : N3879-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

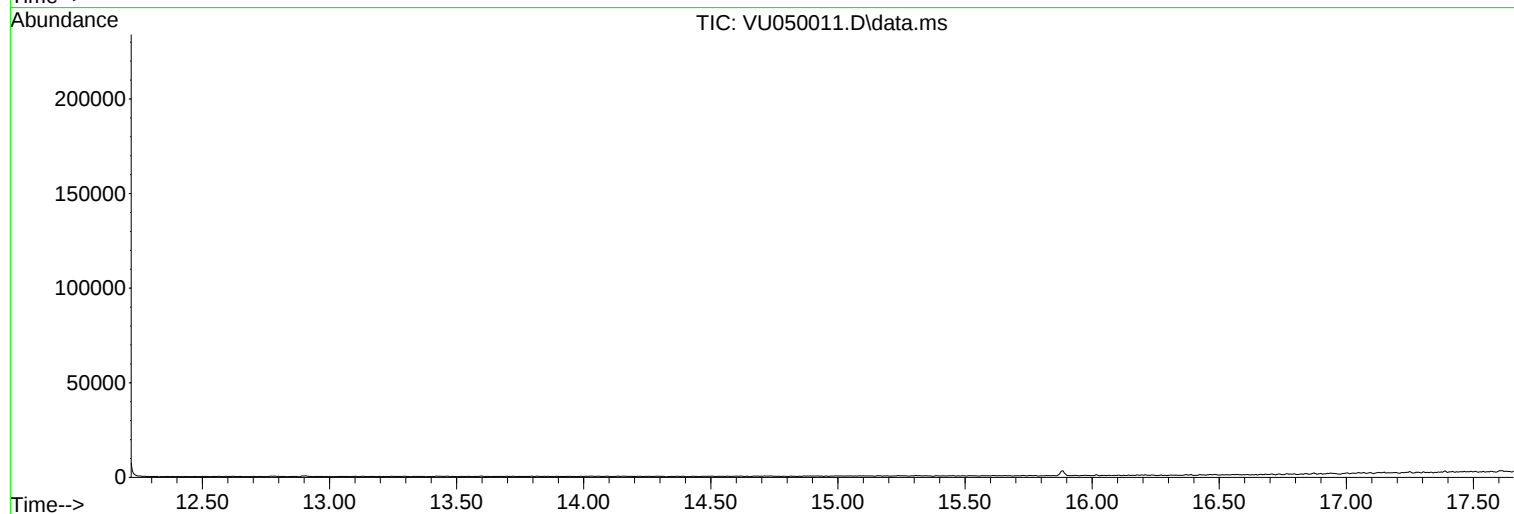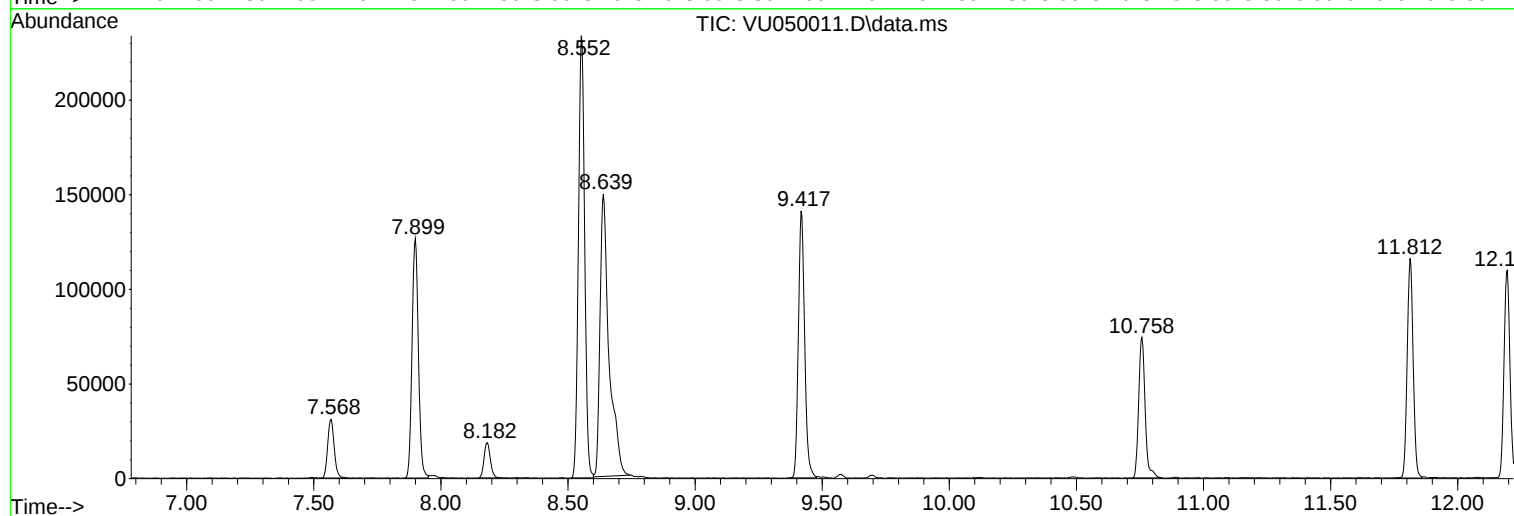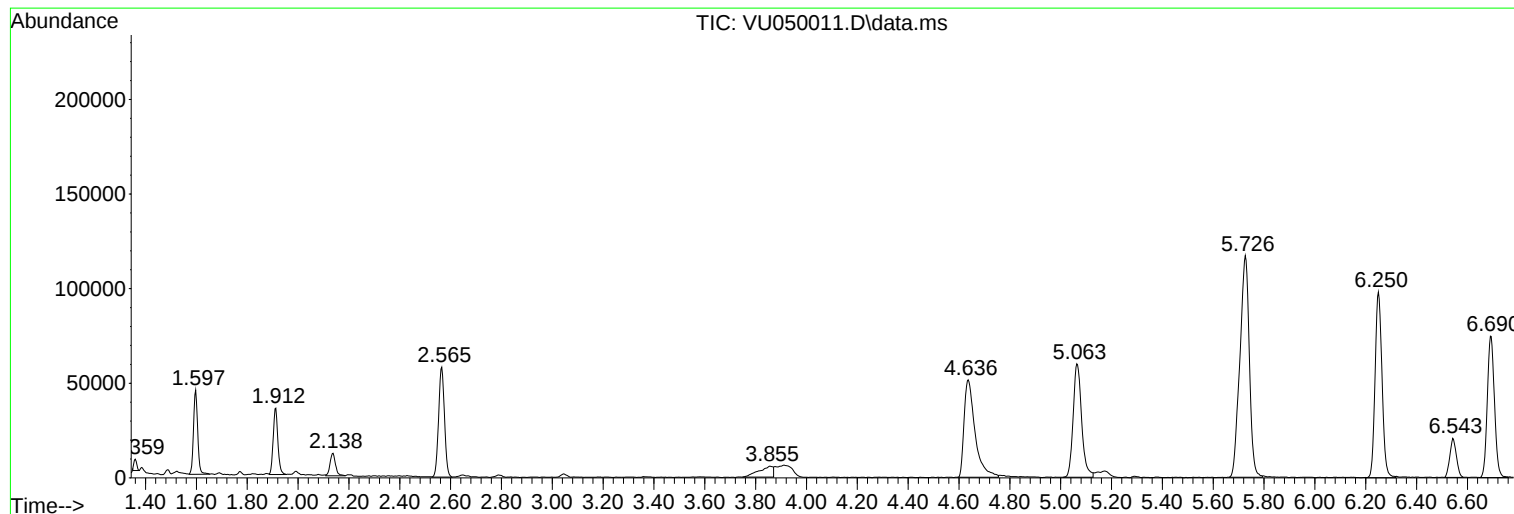

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072822\
Data File : VU050011.D
Acq On : 29 Jul 2022 02:13
Operator : SY/MD
Sample : N3879-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUH6










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.854	0.60 ug/L	22298	1,4-Difluorobenzene	6.250

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1-Propanol	60	C3H8O	000071-23-8	4
2			Acetaldehyde	44	C2H4O	000075-07-0	4
3			Ethylenediamine	60	C2H8N2	000107-15-3	3
4			Acetaldehyde	44	C2H4O	000075-07-0	3
5			Ethylene oxide	44	C2H4O	000075-21-8	3

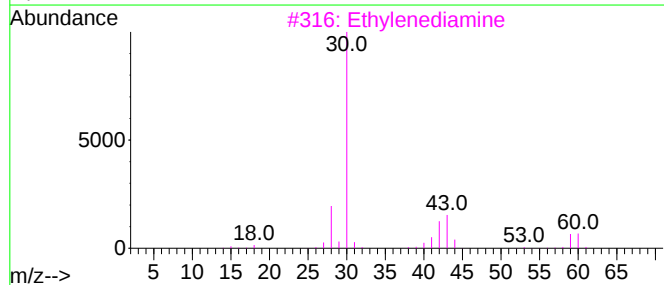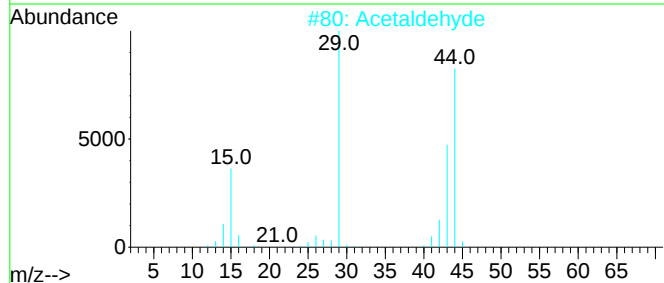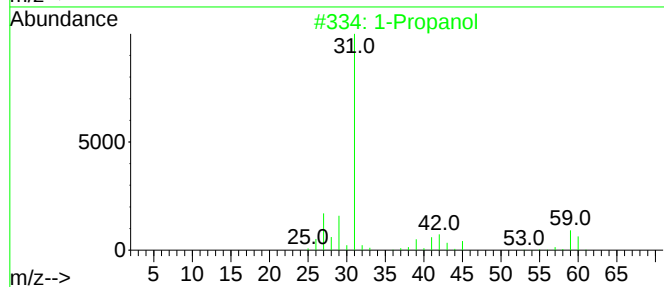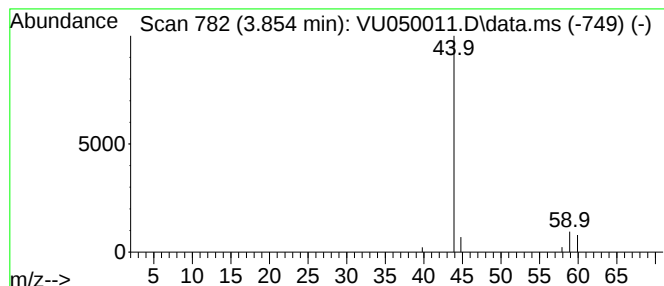

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072822\
Data File : VU050011.D
Acq On : 29 Jul 2022 02:13
Operator : SY/MD
Sample : N3879-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	3.854	0.6	ug/L	22298	1	6.250	187321	5.0