


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072822\
 Data File : VU049979.D
 Acq On : 28 Jul 2022 09:10
 Operator : SY/MD
 Sample : BFB096
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB096

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR072722WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Jul 30 01:40:38 2022

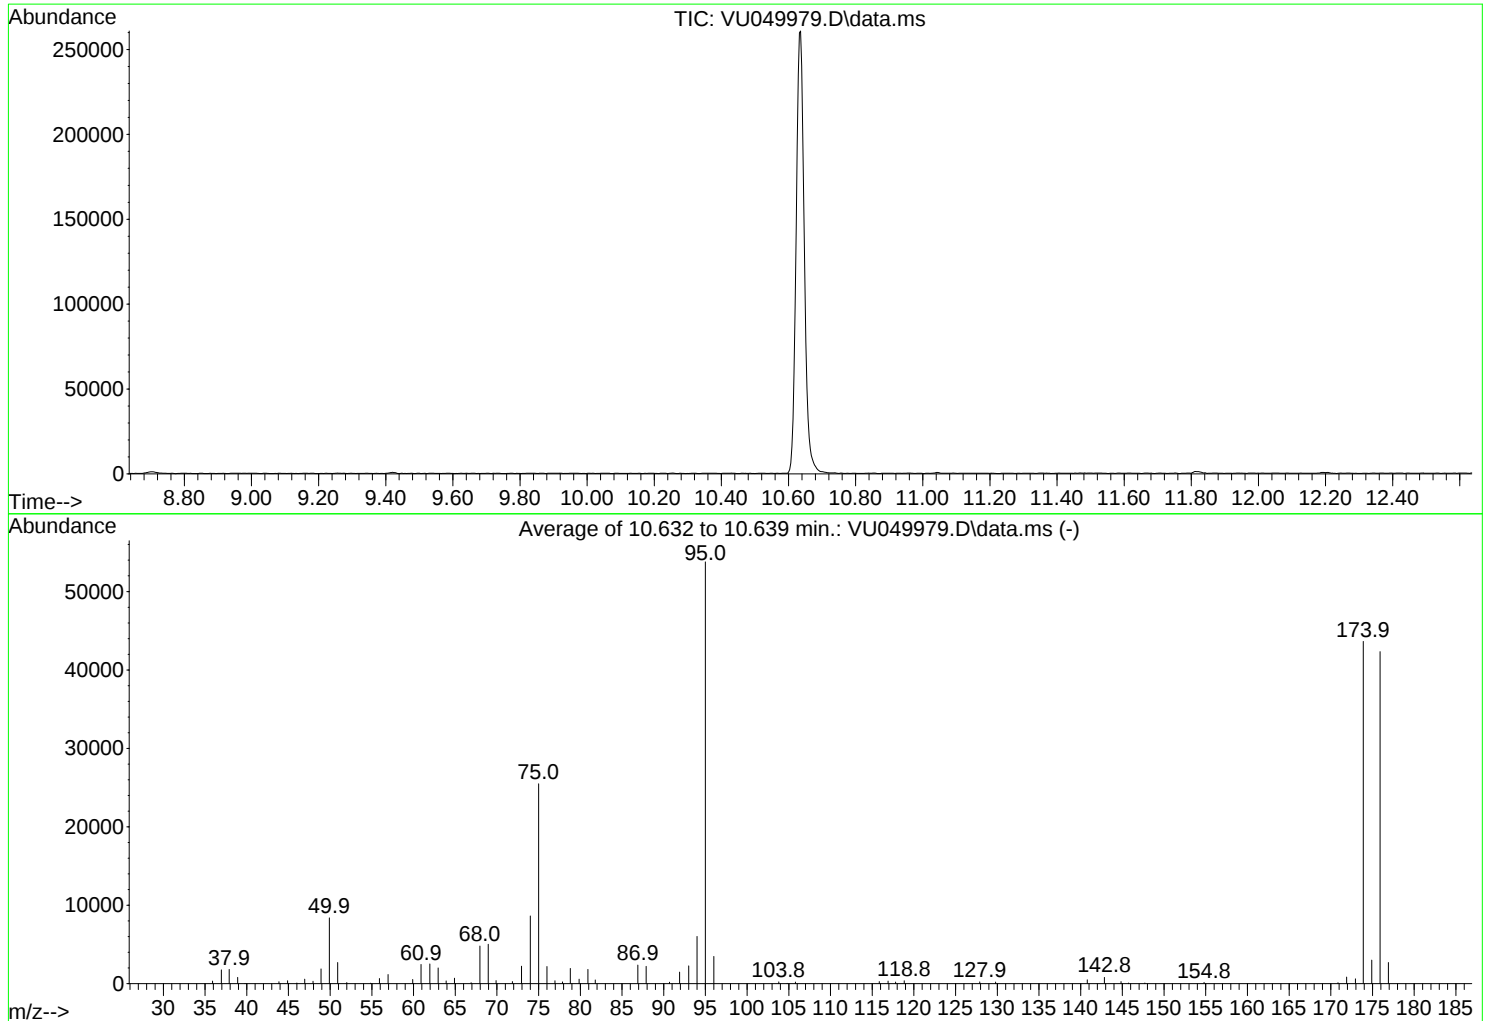

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	8395	PASS
75	95	30	80	47.4	25483	PASS
95	95	100	100	100.0	53789	PASS
96	95	5	9	6.5	3477	PASS
173	174	0.00	2	1.4	610	PASS
174	95	50	120	81.1	43643	PASS
175	174	5	9	6.9	2997	PASS
176	174	95	101	97.0	42336	PASS
177	176	5	9	6.3	2684	PASS

m/z	Abundance
39.90	142.0
43.80	213.0

Instrument :
MSVOA_U
ClientSampleId :
BFB096

m/z	Abundance
35.90	371.0
36.90	1801.0
37.90	1919.0
38.90	786.0
39.80	160.0
43.90	441.0
44.90	419.0
46.00	123.0
47.00	624.0
47.90	294.0
48.90	1927.0
49.90	8733.0
50.90	2844.0
52.10	151.0
55.90	699.0
56.90	1286.0
59.90	580.0
60.90	2573.0
62.00	2595.0
63.00	2073.0
63.90	375.0
64.90	712.0
66.80	145.0
68.00	4874.0
68.90	5264.0
69.90	403.0
71.90	262.0
72.90	2261.0
74.00	8813.0
75.00	26208.0
76.00	2326.0
77.00	397.0
77.80	219.0
78.80	2049.0
79.80	602.0
80.90	1865.0
81.80	433.0
86.90	2435.0
87.90	2295.0
90.70	212.0
91.90	1558.0
93.00	2296.0
94.00	6275.0
95.00	55368.0
96.00	3551.0
103.80	232.0
104.80	127.0
105.80	233.0
115.90	259.0
116.90	380.0
117.80	225.0
118.90	340.0
127.90	215.0
129.80	218.0
140.80	519.0
142.90	809.0
144.90	270.0
147.70	129.0
154.80	172.0
170.80	103.0
171.90	778.0
173.00	647.0
173.90	44184.0
174.90	3133.0
175.90	42552.0
176.90	2742.0

Instrument :
MSVOA_U
ClientSampleId :
BFB096

m/z	Abundance
35.90	339.0
37.00	1814.0
37.90	1850.0
38.90	823.0
39.80	158.0
43.90	460.0
44.90	384.0
46.00	110.0
46.90	585.0
48.00	317.0
48.90	1923.0
49.90	8585.0
50.90	2806.0
52.00	159.0
54.90	104.0
55.90	675.0
57.00	1190.0
59.90	557.0
60.90	2481.0
62.00	2618.0
62.90	2058.0
63.90	352.0
64.90	718.0
66.90	126.0
67.90	4909.0
68.90	5140.0
69.90	395.0
71.80	291.0
73.00	2251.0
74.00	8911.0
75.00	26048.0
76.00	2244.0
76.90	363.0
77.90	242.0
78.80	2007.0
79.90	600.0
80.90	1865.0
81.80	471.0
86.90	2423.0
87.90	2286.0
90.70	198.0
91.90	1509.0
93.00	2328.0
94.00	6188.0
95.00	55536.0
96.00	3615.0
103.80	224.0
105.80	226.0
115.80	289.0
116.90	337.0
117.80	200.0
118.90	386.0
127.90	219.0
129.80	205.0
140.80	519.0
142.90	825.0
144.90	282.0
145.70	107.0
147.70	117.0
154.80	174.0
170.90	121.0
171.90	856.0
172.90	625.0
173.90	44880.0
174.90	3039.0
175.90	43464.0
176.90	2764.0

Instrument :
MSVOA_U
ClientSampleId :
BFB096

m/z	Abundance
35.90	293.0
37.00	1667.0
37.90	1655.0
38.90	810.0
39.80	164.0
43.90	484.0
44.90	330.0
46.90	507.0
48.00	307.0
48.90	1801.0
49.90	7867.0
50.90	2432.0
51.90	132.0
54.80	100.0
55.90	604.0
57.00	1042.0
59.90	473.0
60.90	2275.0
61.90	2336.0
62.90	1893.0
63.90	311.0
64.90	630.0
67.00	119.0
67.90	4576.0
69.00	4676.0
69.90	369.0
71.80	267.0
73.00	2155.0
74.00	8165.0
75.00	24192.0
76.00	1964.0
76.90	325.0
77.90	232.0
78.80	1792.0
79.90	548.0
80.90	1721.0
81.80	511.0
86.90	2245.0
87.90	2013.0
90.70	173.0
91.90	1334.0
93.00	2158.0
94.00	5616.0
95.00	50464.0
96.00	3266.0
103.80	219.0
105.80	181.0
115.80	274.0
116.90	283.0
117.80	167.0
118.80	392.0
127.90	216.0
129.80	179.0
140.80	458.0
142.80	760.0
144.80	266.0
145.80	122.0
154.80	140.0
170.90	122.0
171.90	854.0
172.90	558.0
173.90	41864.0
174.90	2820.0
175.90	40992.0
176.90	2545.0

Instrument :
MSVOA_U
ClientSampleId :
BFB096